




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050537.D
 Acq On : 31 Aug 2022 00:02
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 02:01:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

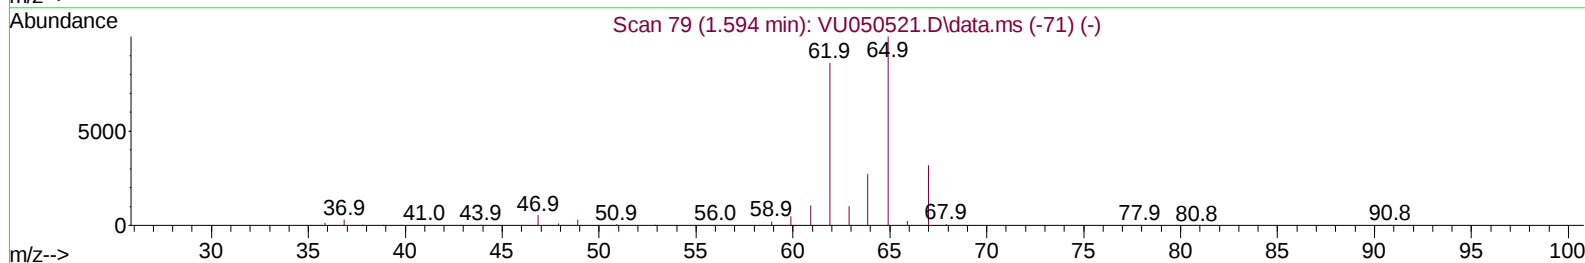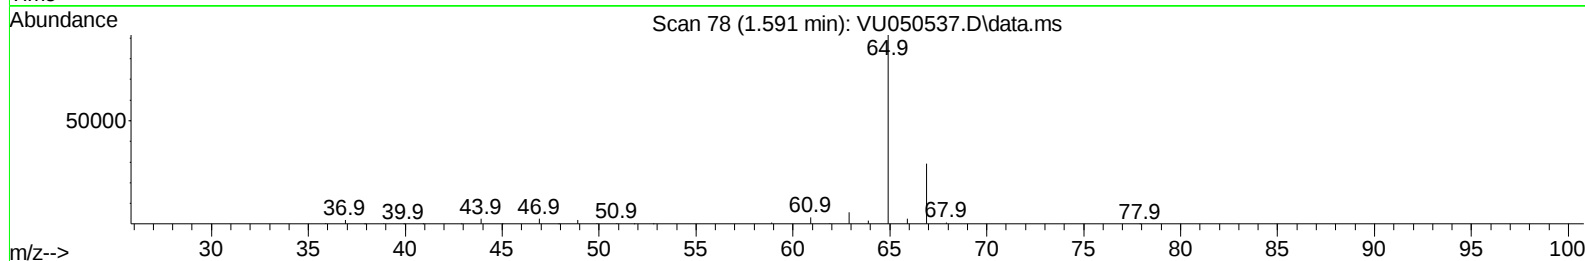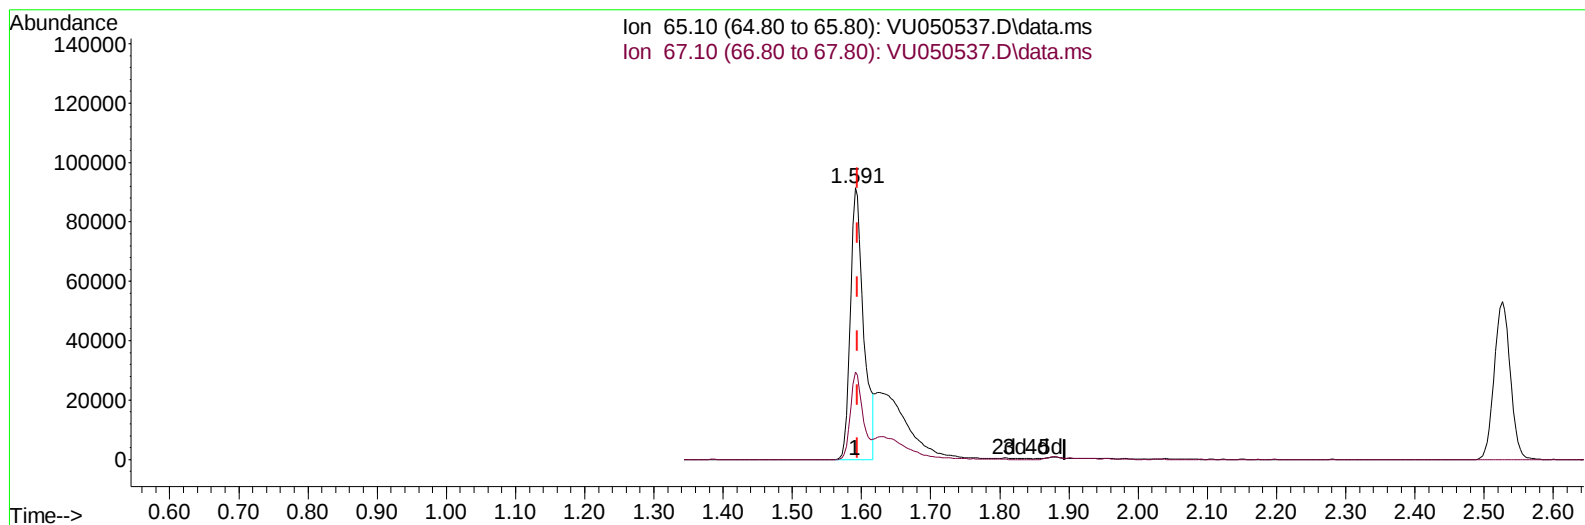

TIC: VU050537.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 49.04 ug/L

response 123711

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	30.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050537.D
 Acq On : 31 Aug 2022 00:02
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 02:01:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

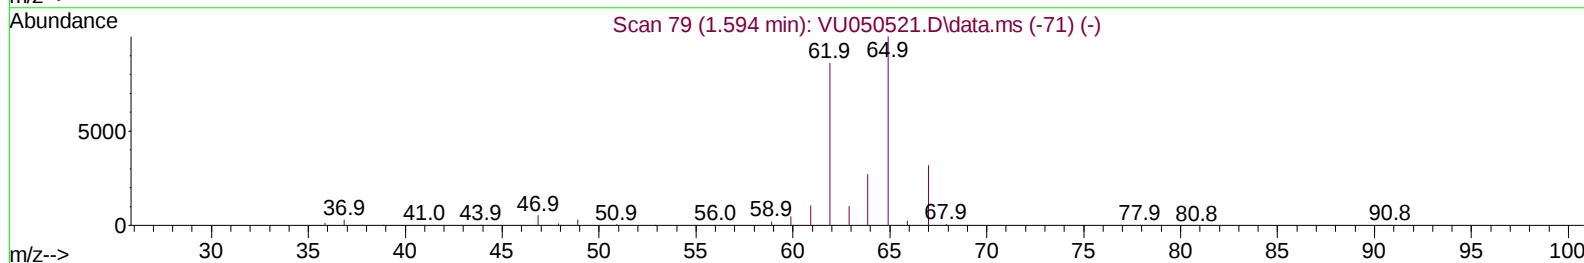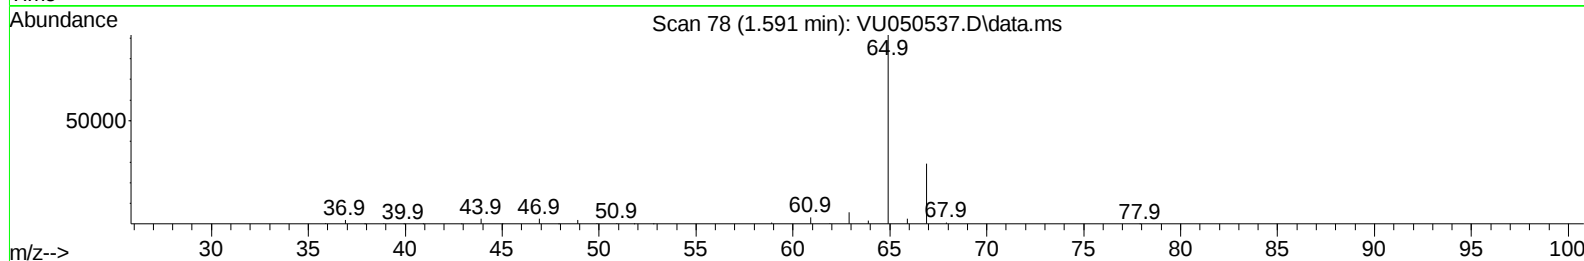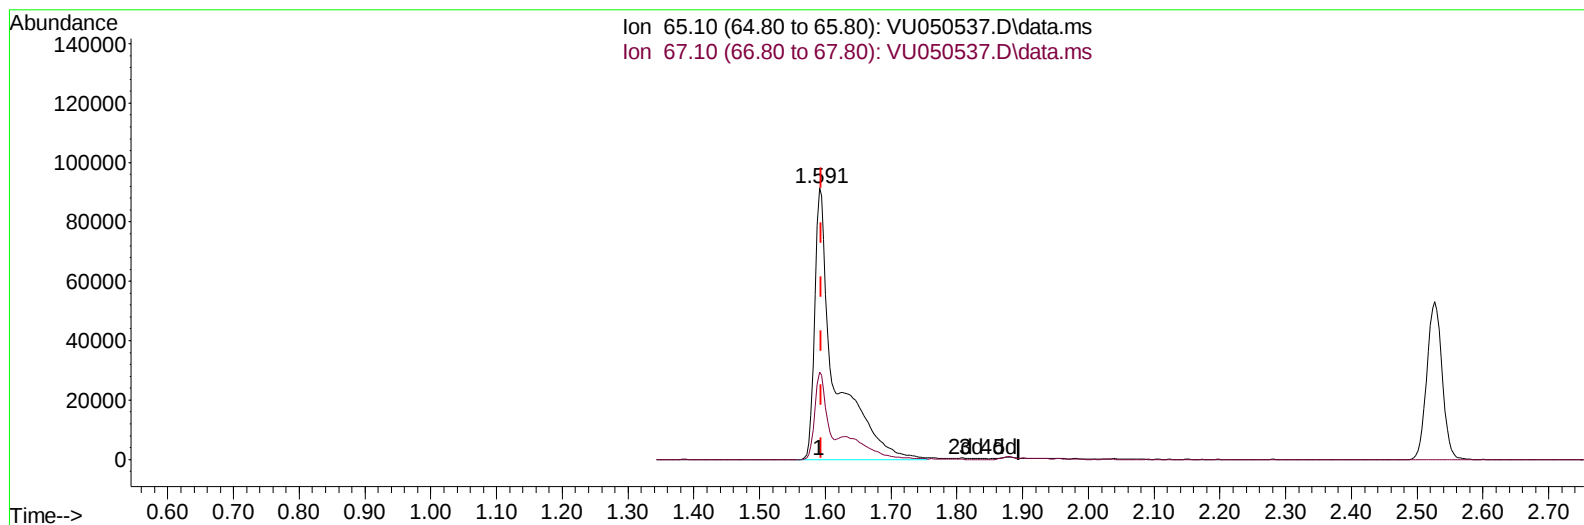

TIC: VU050537.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 78.51 ug/L m

response 198052

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	18.93#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050537.D
 Acq On : 31 Aug 2022 00:02
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 02:01:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	328926	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	328441	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	128804	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.591	65	198052m	78.507	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	157.020%#	
7) Chloroethane-d5	1.877	69	71489	36.347	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	72.700%	
11) 1,1-Dichloroethene-d2	2.526	63	268840	63.117	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	126.240%#	
21) 2-Butanone-d5	4.639	46	436894	198.019	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	198.020%#	
24) Chloroform-d	5.060	84	425852	86.754	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	173.500%#	
26) 1,2-Dichloroethane-d4	5.697	65	288696	90.542	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	181.080%#	
32) Benzene-d6	5.719	84	913177	89.705	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	179.420%#	
36) 1,2-Dichloropropane-d6	6.690	67	307818	90.815	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	181.640%#	
41) Toluene-d8	7.896	98	779662	88.037	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	176.080%#	
43) trans-1,3-Dichloroprop...	8.182	79	101911	74.760	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	149.520%#	
47) 2-Hexanone-d5	8.655	63	286223	233.224	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	233.220%#	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	479958	90.783	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	181.560%#	
66) 1,2-Dichlorobenzene-d4	12.195	152	270091	96.851	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	193.700%#	
Target Compounds						Qvalue
46) Tetrachloroethene	8.552	164	16612	8.673	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050537.D
Acq On : 31 Aug 2022 00:02
Operator : SY/MD
Sample : N4363-11ME
Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVW6ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 02:01:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 31 01:47:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

