

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050541.D
 Acq On : 31 Aug 2022 01:37
 Operator : SY/MD
 Sample : N4345-01ME 100X
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1ME

Quant Time: Aug 31 02:02:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	364918	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	354385	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	129076	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	119856	42.824	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	85.640%		
7) Chloroethane-d5	1.900	69	101820	46.662	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	93.320%		
11) 1,1-Dichloroethene-d2	2.562	63	149950	31.732	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	63.460%		
21) 2-Butanone-d5	4.626	46	198664	81.162	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	81.160%		
24) Chloroform-d	5.063	84	222637	40.882	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	81.760%		
26) 1,2-Dichloroethane-d4	5.700	65	148519	41.985	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	83.980%		
32) Benzene-d6	5.726	84	464676	42.305	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	84.620%		
36) 1,2-Dichloropropane-d6	6.690	67	156543	42.804	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	85.600%		
41) Toluene-d8	7.899	98	376774	39.430	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	78.860%#		
43) trans-1,3-Dichloroprop...	8.179	79	47839	32.525	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	65.040%		
47) 2-Hexanone-d5	8.636	63	109013	82.324	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	82.320%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	218476	38.299	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	76.600%		
66) 1,2-Dichlorobenzene-d4	12.195	152	124494	44.548	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	89.100%		
Target Compounds						
46) Tetrachloroethene	8.552	164	544762	263.609	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050541.D
 Acq On : 31 Aug 2022 01:37
 Operator : SY/MD
 Sample : N4345-01ME 100X
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1ME


Quant Time: Aug 31 02:02:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

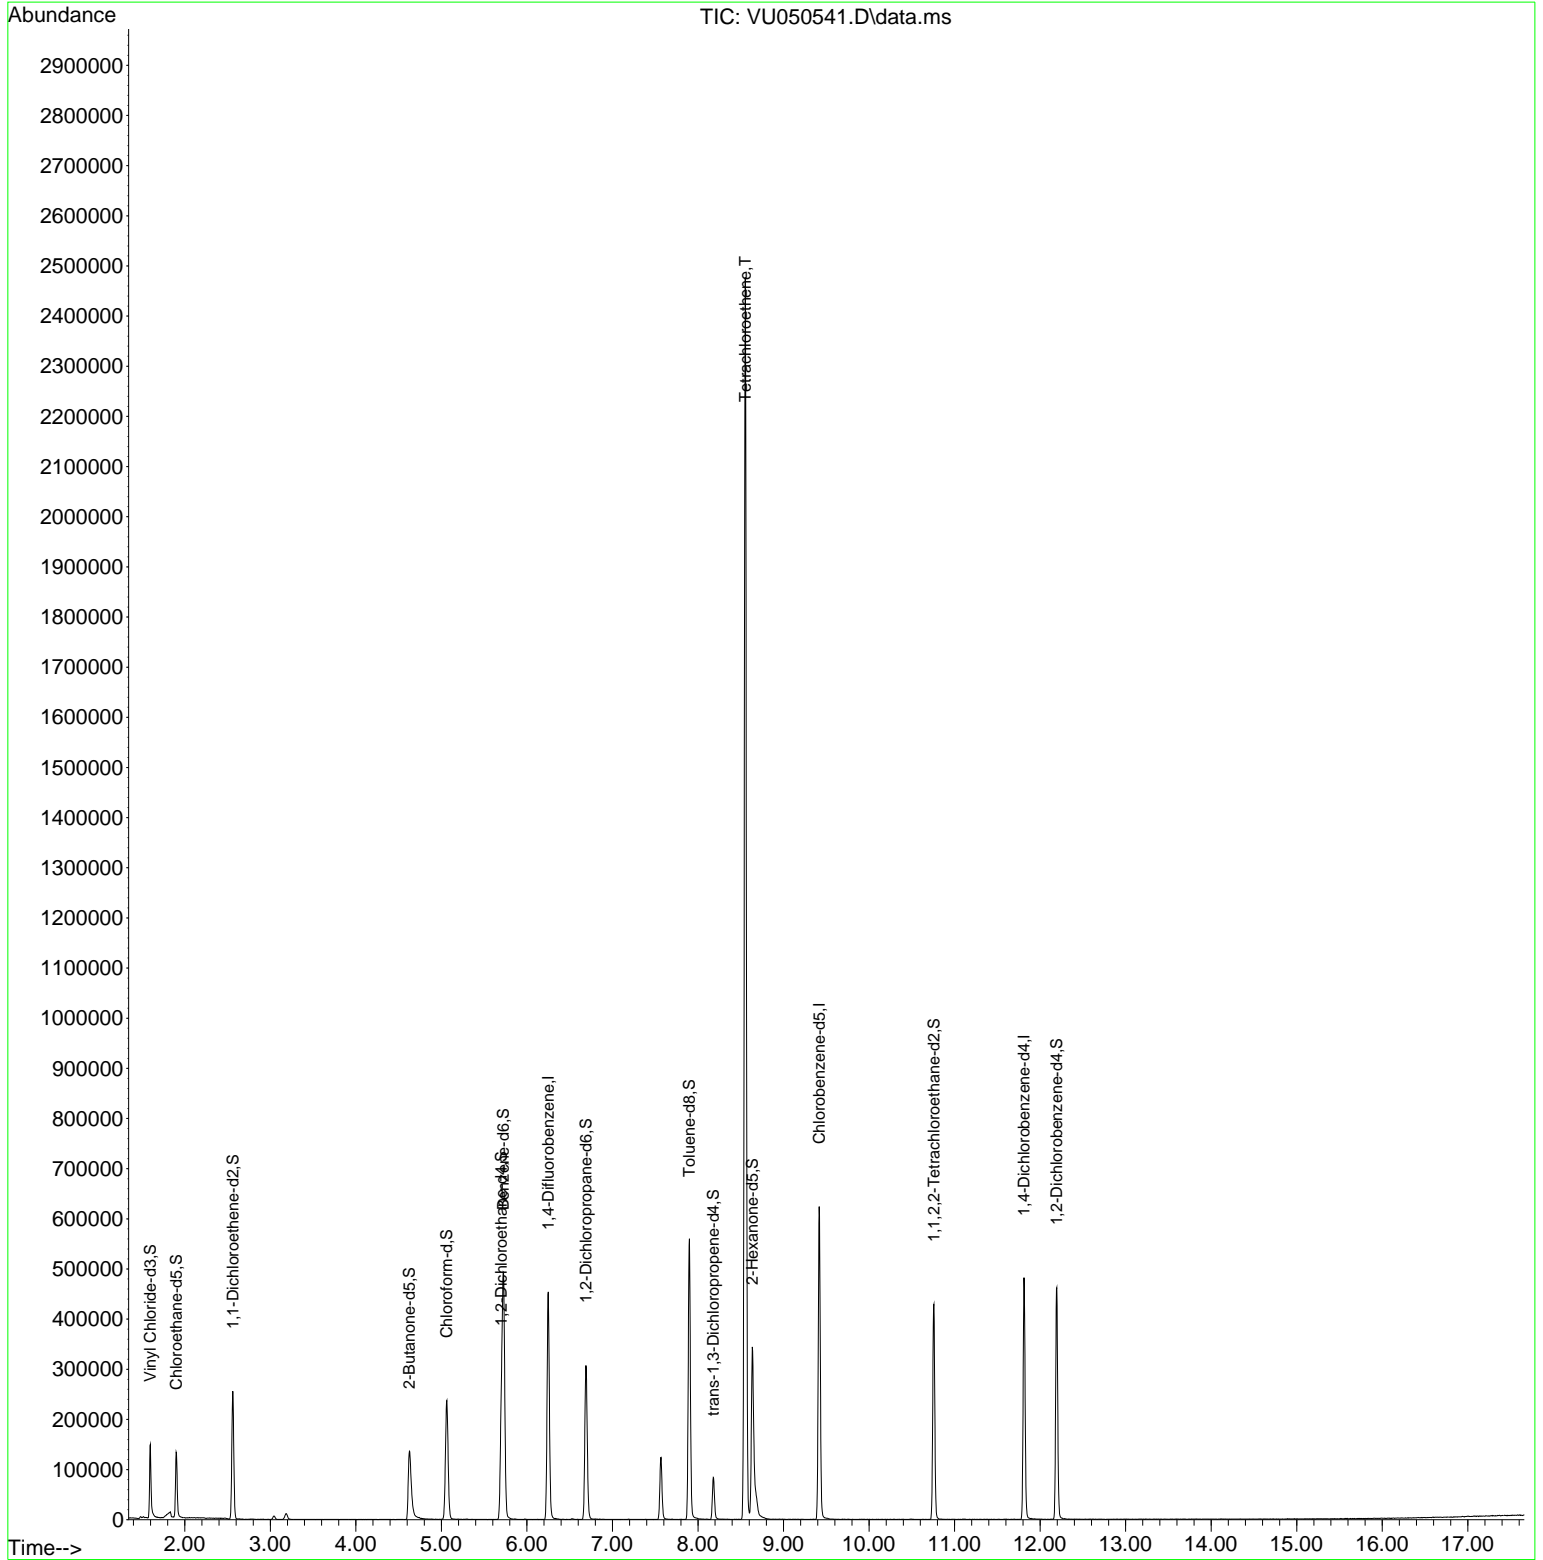

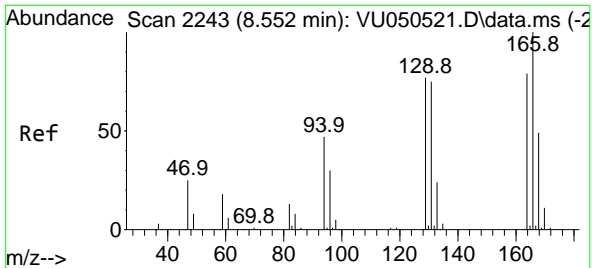

#46
 Tetrachloroethene
 Concen: 263.609 ug/L
 RT: 8.552 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VU050541.D
 Acq: 31 Aug 2022 01:37

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1ME

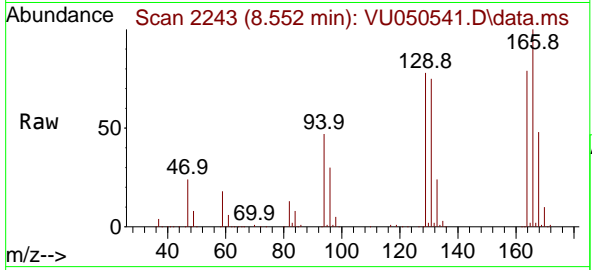

Tgt Ion:164 Resp: 544762

Ion	Ratio	Lower	Upper
164	100		
129	98.7	67.5	125.3
131	94.8	63.8	118.4
166	127.2	87.2	161.9

