

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050540.D
 Acq On : 31 Aug 2022 01:13
 Operator : SY/MD
 Sample : N4345-17ME 50X
 Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	103	rBV	136208	182280	13.00%	1.744%
2	1.893	165	172	193	rVB	128513	179055	12.77%	1.713%
3	2.559	367	379	395	rVB	248263	398728	28.44%	3.815%
4	2.964	501	505	509	rBV2	317	287	0.02%	0.003%
5	3.041	519	529	540	rVB2	7571	13581	0.97%	0.130%
6	3.112	546	551	552	rBV2	229	189	0.01%	0.002%
7	3.182	558	573	595	rBV	61289	150118	10.71%	1.436%
8	3.372	630	632	634	rBV	218	100	0.01%	0.001%
9	3.497	668	671	676	rVB2	239	236	0.02%	0.002%
10	3.523	676	679	682	rVB	447	253	0.02%	0.002%
11	3.546	682	686	689	rBV2	146	138	0.01%	0.001%
12	3.568	690	693	695	rBV2	169	121	0.01%	0.001%
13	3.661	719	722	726	rVB	165	128	0.01%	0.001%
14	3.687	726	730	732	rBV2	242	177	0.01%	0.002%
15	3.777	754	758	764	rVB2	304	318	0.02%	0.003%
16	3.806	764	767	770	rBV3	208	128	0.01%	0.001%
17	3.822	770	772	774	rBV	245	135	0.01%	0.001%
18	3.983	818	822	829	rVB2	208	232	0.02%	0.002%
19	4.018	830	833	836	rVB2	175	102	0.01%	0.001%
20	4.038	836	839	842	rBV2	194	147	0.01%	0.001%
21	4.150	872	874	877	rVB	209	108	0.01%	0.001%
22	4.211	890	893	897	rBV	212	173	0.01%	0.002%
23	4.234	897	900	902	rBV2	143	103	0.01%	0.001%
24	4.288	913	917	922	rVB2	289	253	0.02%	0.002%
25	4.420	955	958	961	rVB2	160	89	0.01%	0.001%
26	4.443	962	965	968	rBV	172	112	0.01%	0.001%
27	4.504	981	984	987	rBV2	229	161	0.01%	0.002%
28	4.629	1006	1023	1073	rBV2	148437	433579	30.93%	4.149%
29	5.063	1141	1158	1187	rBV	244823	540909	38.58%	5.176%
30	5.202	1198	1201	1202	rBV	491	274	0.02%	0.003%
31	5.275	1220	1224	1225	rBV	608	392	0.03%	0.004%
32	5.411	1263	1266	1268	rBV	190	112	0.01%	0.001%
33	5.439	1272	1275	1279	rBV2	191	150	0.01%	0.001%
34	5.523	1298	1301	1308	rVB2	262	257	0.02%	0.002%
35	5.558	1308	1312	1317	rBV2	167	146	0.01%	0.001%
36	5.600	1322	1325	1327	rBV	288	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050540.D
 Acq On : 31 Aug 2022 01:13
 Operator : SY/MD
 Sample : N4345-17ME 50X
 Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	5.645	1336	1339	1341	rBV2	175	108	0.01%	0.001%
38	5.722	1341	1363	1388	rBV2	524456	1401873	100.00%	13.414%
39	6.050	1461	1465	1470	rVB3	350	283	0.02%	0.003%
40	6.099	1475	1480	1481	rBV	120	95	0.01%	0.001%
41	6.140	1491	1493	1497	rVB2	203	127	0.01%	0.001%
42	6.250	1510	1527	1555	rBV	440119	842106	60.07%	8.058%
43	6.536	1604	1616	1625	rBV9	1723	3503	0.25%	0.034%
44	6.571	1625	1627	1630	rVB2	217	96	0.01%	0.001%
45	6.591	1630	1633	1635	rBV	334	256	0.02%	0.002%
46	6.690	1650	1664	1689	rBV	332657	649834	46.35%	6.218%
47	6.967	1747	1750	1752	rBV	257	172	0.01%	0.002%
48	7.250	1835	1838	1844	rVB	283	206	0.01%	0.002%
49	7.291	1849	1851	1854	rVV2	237	118	0.01%	0.001%
50	7.359	1869	1872	1874	rBV	232	148	0.01%	0.001%
51	7.439	1893	1897	1900	rBV	171	137	0.01%	0.001%
52	7.510	1914	1919	1924	rVB2	356	206	0.01%	0.002%
53	7.568	1924	1937	1960	rBV	128850	231363	16.50%	2.214%
54	7.697	1974	1977	1978	rBV3	350	171	0.01%	0.002%
55	7.742	1989	1991	1995	rVB	251	167	0.01%	0.002%
56	7.771	1995	2000	2004	rBV2	362	414	0.03%	0.004%
57	7.899	2026	2040	2064	rBV	562363	980206	69.92%	9.379%
58	8.179	2116	2127	2145	rBV	86356	148035	10.56%	1.416%
59	8.398	2193	2195	2198	rBV2	263	188	0.01%	0.002%
60	8.462	2211	2215	2221	rBV4	329	321	0.02%	0.003%
61	8.552	2231	2243	2257	rBV	177211	296036	21.12%	2.833%
62	8.639	2258	2270	2313	rBV2	348774	746522	53.25%	7.143%
63	8.889	2345	2348	2351	rBV3	379	303	0.02%	0.003%
64	9.031	2390	2392	2394	rBV	253	100	0.01%	0.001%
65	9.047	2394	2397	2400	rBV	331	218	0.02%	0.002%
66	9.089	2407	2410	2412	rBV2	271	220	0.02%	0.002%
67	9.163	2431	2433	2437	rBV	167	124	0.01%	0.001%
68	9.230	2451	2454	2457	rVB	355	186	0.01%	0.002%
69	9.301	2472	2476	2481	rBV2	199	192	0.01%	0.002%
70	9.417	2498	2512	2538	rBV	605479	1008109	71.91%	9.646%
71	9.645	2580	2583	2587	rVB3	213	126	0.01%	0.001%
72	9.677	2589	2593	2596	rBV	290	232	0.02%	0.002%
73	9.722	2605	2607	2610	rBV2	240	94	0.01%	0.001%
74	9.787	2623	2627	2630	rBV	258	187	0.01%	0.002%
75	9.838	2640	2643	2649	rVB2	325	268	0.02%	0.003%
76	9.867	2649	2652	2655	rBV2	177	97	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050540.D
 Acq On : 31 Aug 2022 01:13
 Operator : SY/MD
 Sample : N4345-17ME 50X
 Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	9.931	2670	2672	2675	rVB2	395	219	0.02%	0.002%
78	9.951	2675	2678	2680	rBV3	388	276	0.02%	0.003%
79	10.018	2697	2699	2701	rBV	189	94	0.01%	0.001%
80	10.031	2701	2703	2707	rVB2	237	134	0.01%	0.001%
81	10.092	2718	2722	2726	rBV3	288	258	0.02%	0.002%
82	10.311	2787	2790	2794	rBV2	220	172	0.01%	0.002%
83	10.346	2798	2801	2807	rVB	228	196	0.01%	0.002%
84	10.430	2825	2827	2832	rVB	359	269	0.02%	0.003%
85	10.510	2849	2852	2854	rBV	154	84	0.01%	0.001%
86	10.549	2861	2864	2866	rVB2	263	171	0.01%	0.002%
87	10.606	2879	2882	2884	rBV2	186	139	0.01%	0.001%
88	10.713	2912	2915	2916	rBV	264	161	0.01%	0.002%
89	10.758	2916	2929	2949	rVV	455320	733133	52.30%	7.015%
90	11.041	3013	3017	3018	rBV2	345	234	0.02%	0.002%
91	11.073	3024	3027	3030	rBV2	344	319	0.02%	0.003%
92	11.118	3037	3041	3051	rVB5	961	1296	0.09%	0.012%
93	11.169	3051	3057	3061	rBV2	299	404	0.03%	0.004%
94	11.462	3145	3148	3151	rBV	305	214	0.02%	0.002%
95	11.616	3193	3196	3199	rBV3	327	225	0.02%	0.002%
96	11.664	3208	3211	3220	rBV2	270	419	0.03%	0.004%
97	11.812	3244	3257	3273	rBV	457474	729859	52.06%	6.984%
98	12.195	3362	3376	3397	rBV	466428	765504	54.61%	7.325%
99	12.938	3604	3607	3608	rBV	383	174	0.01%	0.002%
100	13.063	3643	3646	3648	rBV	442	373	0.03%	0.004%


Sum of corrected areas: 10450944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050540.D
Acq On : 31 Aug 2022 01:13
Operator : SY/MD
Sample : N4345-17ME 50X
Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

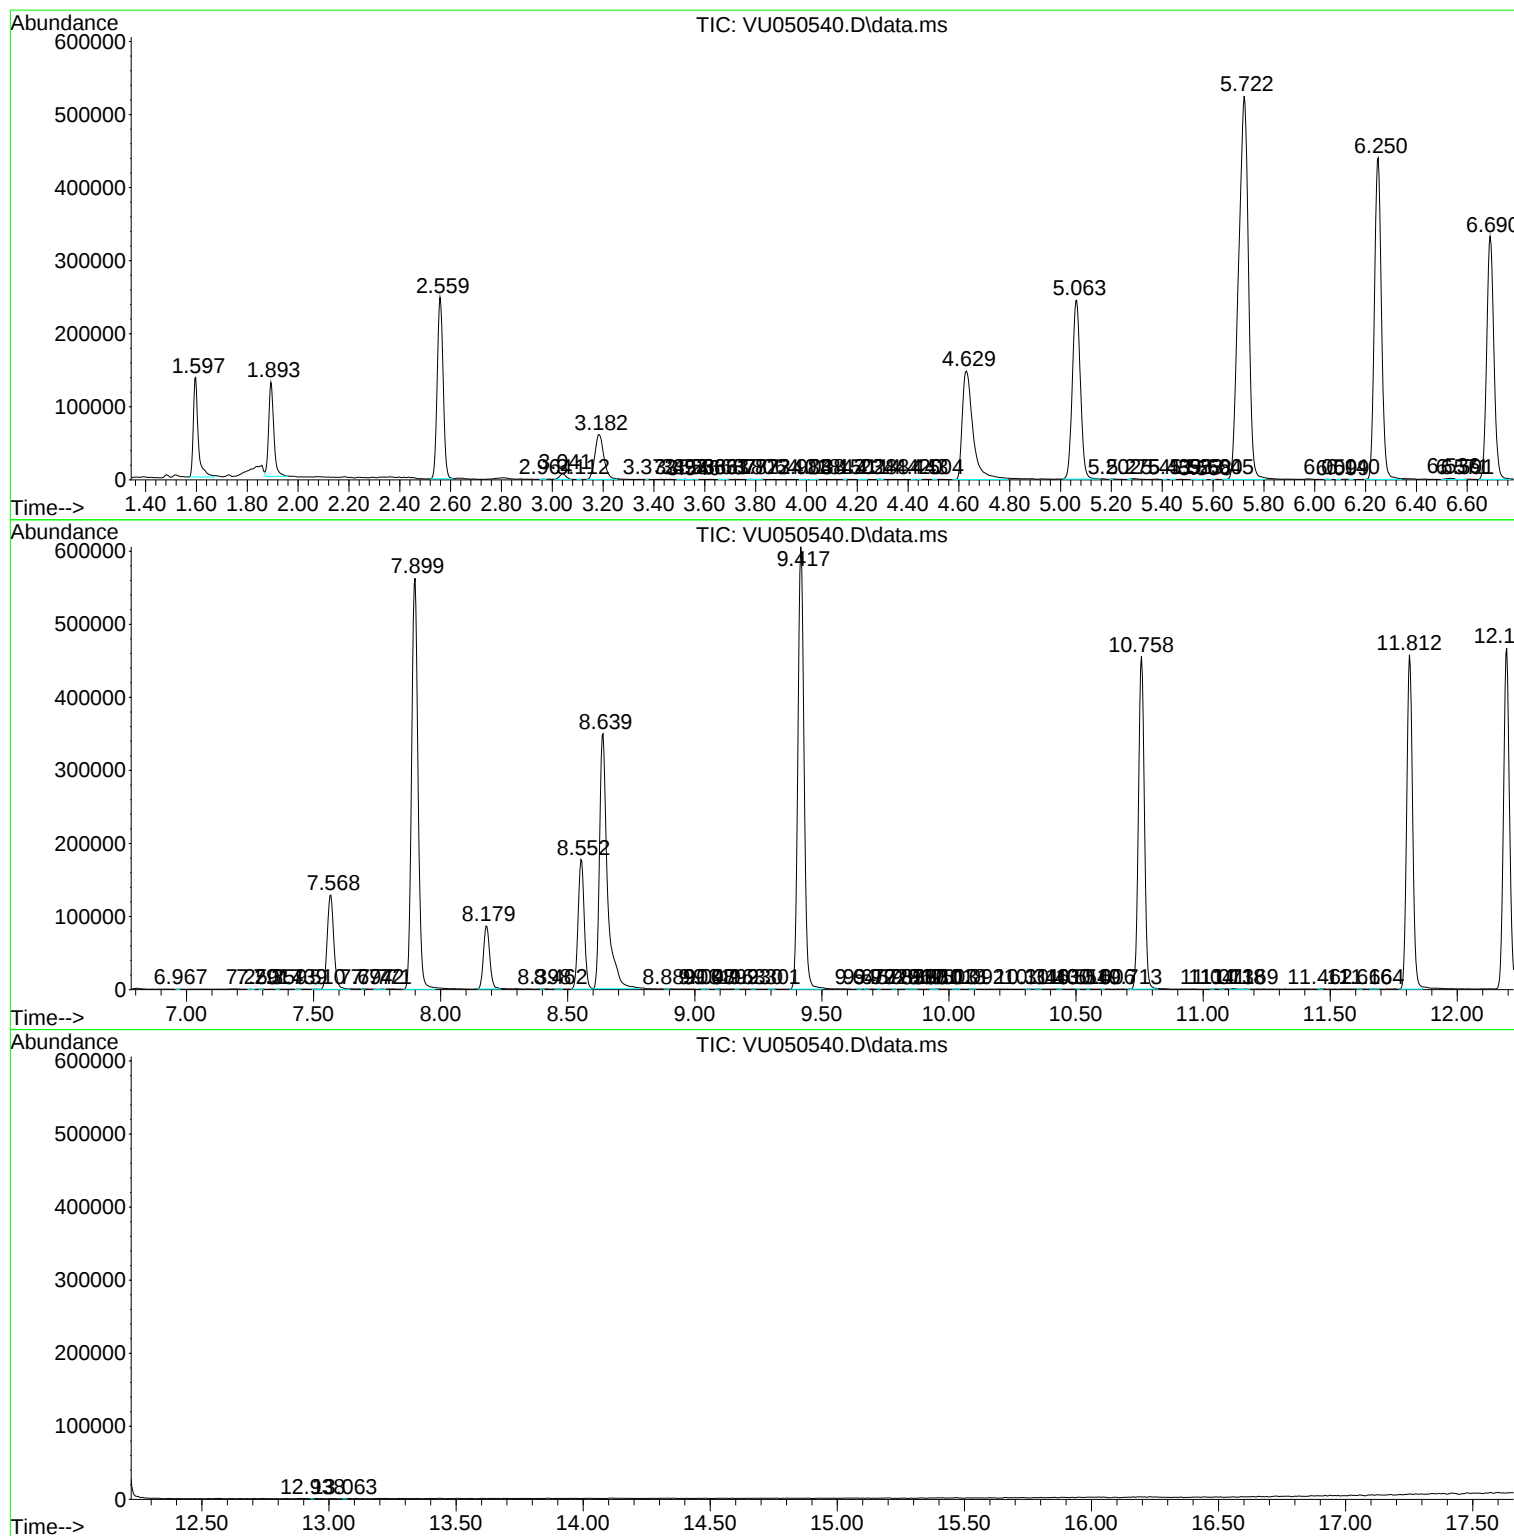

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050540.D
Acq On : 31 Aug 2022 01:13
Operator : SY/MD
Sample : N4345-17ME 50X
Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050540.D
Acq On : 31 Aug 2022 01:13
Operator : SY/MD
Sample : N4345-17ME 50X
Misc : 5.66g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
