

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050543.D
 Acq On : 31 Aug 2022 02:24
 Operator : SY/MD
 Sample : N4345-03ME 100X
 Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV3	2688	3294	0.24%	0.030%
2	1.520	51	56	63	rVV2	2405	3530	0.26%	0.032%
3	1.597	72	80	99	rBV	155974	195351	14.23%	1.760%
4	1.903	167	175	195	rVB	137641	184976	13.48%	1.666%
5	2.562	368	380	395	rBV	264170	424274	30.91%	3.822%
6	2.838	464	466	469	rVB	295	154	0.01%	0.001%
7	2.861	469	473	479	rBV2	465	628	0.05%	0.006%
8	3.044	520	530	543	rVB2	7052	12137	0.88%	0.109%
9	3.096	543	546	549	rBV2	209	160	0.01%	0.001%
10	3.131	553	557	560	rBV2	238	233	0.02%	0.002%
11	3.186	560	574	590	rVB	13994	31370	2.29%	0.283%
12	3.317	610	615	622	rBV2	219	352	0.03%	0.003%
13	3.443	651	654	658	rBV	239	210	0.02%	0.002%
14	3.597	698	702	704	rBV	191	191	0.01%	0.002%
15	3.652	715	719	721	rBV2	311	236	0.02%	0.002%
16	3.706	733	736	740	rVB2	316	184	0.01%	0.002%
17	3.748	747	749	754	rBV2	263	172	0.01%	0.002%
18	3.858	780	783	787	rVB	276	213	0.02%	0.002%
19	3.886	787	792	795	rBV2	279	291	0.02%	0.003%
20	3.922	796	803	806	rBV	288	294	0.02%	0.003%
21	3.970	814	818	820	rBV	263	223	0.02%	0.002%
22	4.060	841	846	848	rBV2	232	208	0.02%	0.002%
23	4.221	889	896	897	rBV2	252	219	0.02%	0.002%
24	4.423	956	959	964	rVV2	225	237	0.02%	0.002%
25	4.449	964	967	970	rVB	346	200	0.01%	0.002%
26	4.520	983	989	994	rBV2	298	466	0.03%	0.004%
27	4.626	1009	1022	1051	rBV	144363	378345	27.57%	3.408%
28	5.063	1141	1158	1183	rBV	242086	529334	38.57%	4.768%
29	5.214	1203	1205	1215	rVB5	651	739	0.05%	0.007%
30	5.282	1218	1226	1228	rBV4	896	1031	0.08%	0.009%
31	5.324	1237	1239	1245	rVB2	244	189	0.01%	0.002%
32	5.375	1249	1255	1257	rVV4	396	351	0.03%	0.003%
33	5.722	1342	1363	1387	rBV2	509662	1372418	100.00%	12.363%
34	5.983	1440	1444	1445	rBV	531	330	0.02%	0.003%
35	6.018	1453	1455	1461	rBV2	424	361	0.03%	0.003%
36	6.047	1461	1464	1466	rBV2	289	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050543.D
 Acq On : 31 Aug 2022 02:24
 Operator : SY/MD
 Sample : N4345-03ME 100X
 Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.169	1498	1502	1505	rVB2	212	153	0.01%	0.001%
38	6.250	1512	1527	1554	rBV	441435	839515	61.17%	7.562%
39	6.491	1599	1602	1607	rBV2	312	272	0.02%	0.002%
40	6.533	1607	1615	1620	rVV5	1335	2203	0.16%	0.020%
41	6.555	1620	1622	1626	rVV2	362	190	0.01%	0.002%
42	6.594	1630	1634	1639	rVB2	245	219	0.02%	0.002%
43	6.690	1648	1664	1689	rBV	323979	635472	46.30%	5.724%
44	6.803	1697	1699	1702	rBV2	547	241	0.02%	0.002%
45	7.115	1793	1796	1799	rBV	237	156	0.01%	0.001%
46	7.189	1816	1819	1825	rVV3	359	325	0.02%	0.003%
47	7.391	1879	1882	1887	rVB	253	175	0.01%	0.002%
48	7.423	1888	1892	1896	rBV2	225	213	0.02%	0.002%
49	7.565	1923	1936	1954	rBV2	122978	220491	16.07%	1.986%
50	7.648	1960	1962	1964	rBV2	371	215	0.02%	0.002%
51	7.706	1976	1980	1985	rBV4	364	344	0.03%	0.003%
52	7.899	2025	2040	2070	rBV	569454	995940	72.57%	8.971%
53	8.134	2110	2113	2116	rBV2	256	220	0.02%	0.002%
54	8.179	2116	2127	2143	rBV	82886	142275	10.37%	1.282%
55	8.552	2230	2243	2258	rBV	638579	1079710	78.67%	9.726%
56	8.635	2258	2269	2319	rVB3	325185	753007	54.87%	6.783%
57	8.848	2333	2335	2338	rVB2	424	199	0.01%	0.002%
58	8.870	2338	2342	2344	rBV2	440	335	0.02%	0.003%
59	8.941	2360	2364	2368	rVB3	353	347	0.03%	0.003%
60	8.970	2368	2373	2374	rBV2	348	292	0.02%	0.003%
61	9.025	2388	2390	2393	rVB2	414	250	0.02%	0.002%
62	9.076	2403	2406	2409	rBV2	209	171	0.01%	0.002%
63	9.417	2499	2512	2541	rVV	604593	1021908	74.46%	9.205%
64	9.626	2575	2577	2580	rVB	258	175	0.01%	0.002%
65	9.668	2584	2590	2596	rBV2	232	333	0.02%	0.003%
66	9.832	2637	2641	2643	rBV	240	189	0.01%	0.002%
67	9.844	2643	2645	2648	rVB	339	166	0.01%	0.001%
68	9.864	2648	2651	2652	rBV2	218	154	0.01%	0.001%
69	9.983	2685	2688	2692	rBV2	255	170	0.01%	0.002%
70	10.018	2695	2699	2702	rBV2	287	272	0.02%	0.002%
71	10.066	2709	2714	2718	rVB2	242	242	0.02%	0.002%
72	10.111	2725	2728	2729	rBV2	275	181	0.01%	0.002%
73	10.143	2735	2738	2741	rBV	361	215	0.02%	0.002%
74	10.449	2830	2833	2838	rBV2	340	256	0.02%	0.002%
75	10.754	2916	2928	2948	rBV	438230	721587	52.58%	6.500%
76	10.851	2956	2958	2960	rBV2	346	179	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050543.D
 Acq On : 31 Aug 2022 02:24
 Operator : SY/MD
 Sample : N4345-03ME 100X
 Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.880	2964	2967	2968	rBV	432	196	0.01%	0.002%
78	10.947	2986	2988	2994	rVB3	320	233	0.02%	0.002%
79	11.002	3002	3005	3010	rVB2	402	358	0.03%	0.003%
80	11.114	3038	3040	3043	rVV	340	206	0.02%	0.002%
81	11.645	3201	3205	3207	rBV3	330	253	0.02%	0.002%
82	11.812	3244	3257	3279	rBV	467272	755703	55.06%	6.807%
83	12.195	3362	3376	3398	rBV	468138	776699	56.59%	6.996%
84	12.661	3518	3521	3525	rVB3	316	231	0.02%	0.002%
85	12.684	3525	3528	3531	rBV	426	290	0.02%	0.003%
86	12.796	3560	3563	3566	rVB2	309	156	0.01%	0.001%
87	13.102	3654	3658	3665	rVB2	489	552	0.04%	0.005%
88	13.130	3665	3667	3670	rBV	371	237	0.02%	0.002%
89	13.192	3682	3686	3689	rBV2	367	324	0.02%	0.003%
90	13.237	3699	3700	3703	rBV2	257	155	0.01%	0.001%
91	13.253	3703	3705	3709	rVB2	307	190	0.01%	0.002%
92	13.314	3718	3724	3730	rBV3	424	563	0.04%	0.005%
93	13.401	3746	3751	3753	rBV3	350	248	0.02%	0.002%
94	13.442	3762	3764	3765	rBV	349	153	0.01%	0.001%
95	13.748	3850	3859	3863	rBV3	433	714	0.05%	0.006%
96	13.819	3878	3881	3883	rBV	366	231	0.02%	0.002%
97	13.960	3921	3925	3926	rBV2	349	251	0.02%	0.002%
98	14.011	3938	3941	3943	rBV	436	289	0.02%	0.003%
99	14.507	4091	4095	4099	rBV3	549	553	0.04%	0.005%
100	14.915	4218	4222	4227	rBV3	512	485	0.04%	0.004%




Sum of corrected areas: 11101317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050543.D
Acq On : 31 Aug 2022 02:24
Operator : SY/MD
Sample : N4345-03ME 100X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

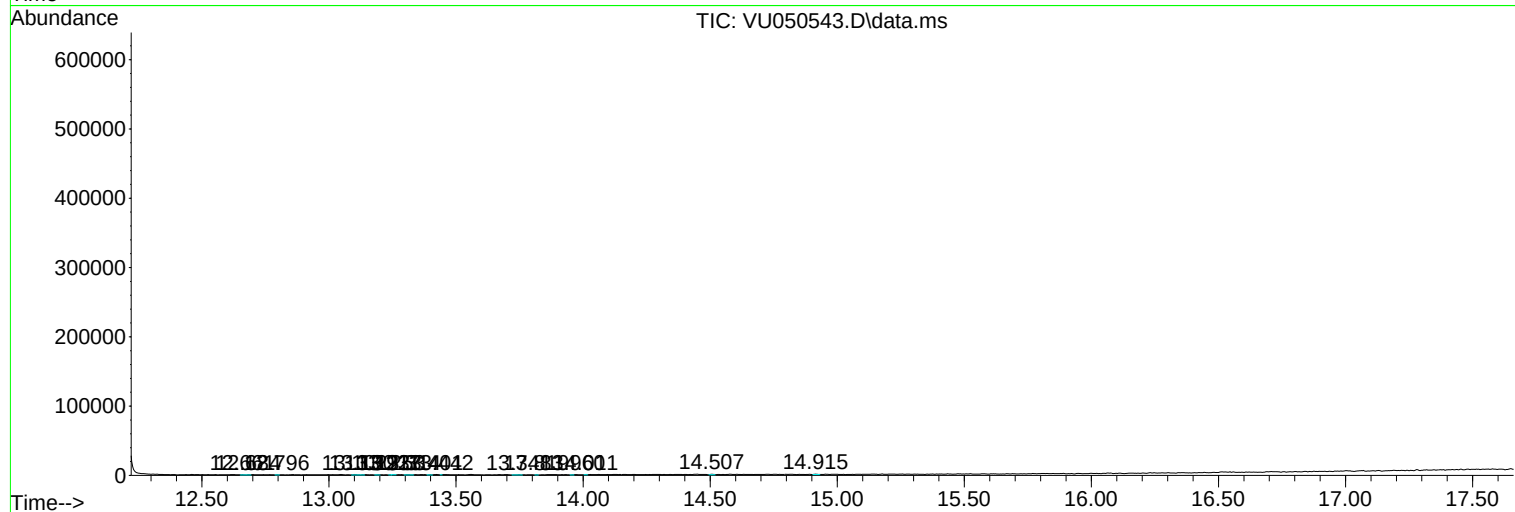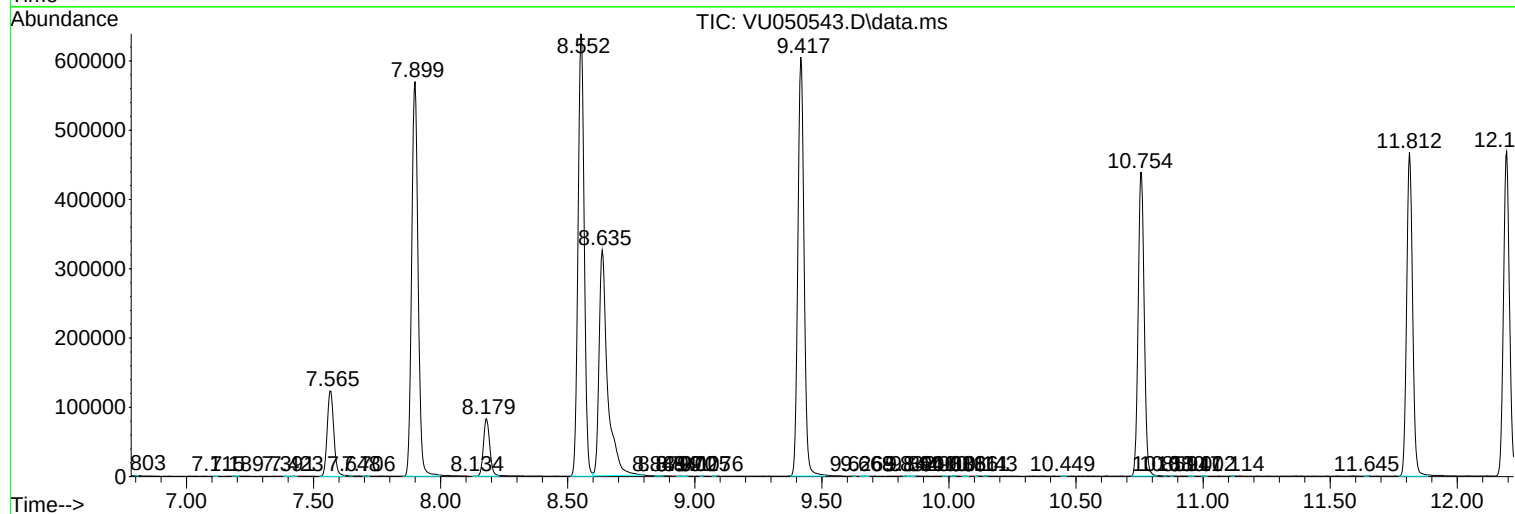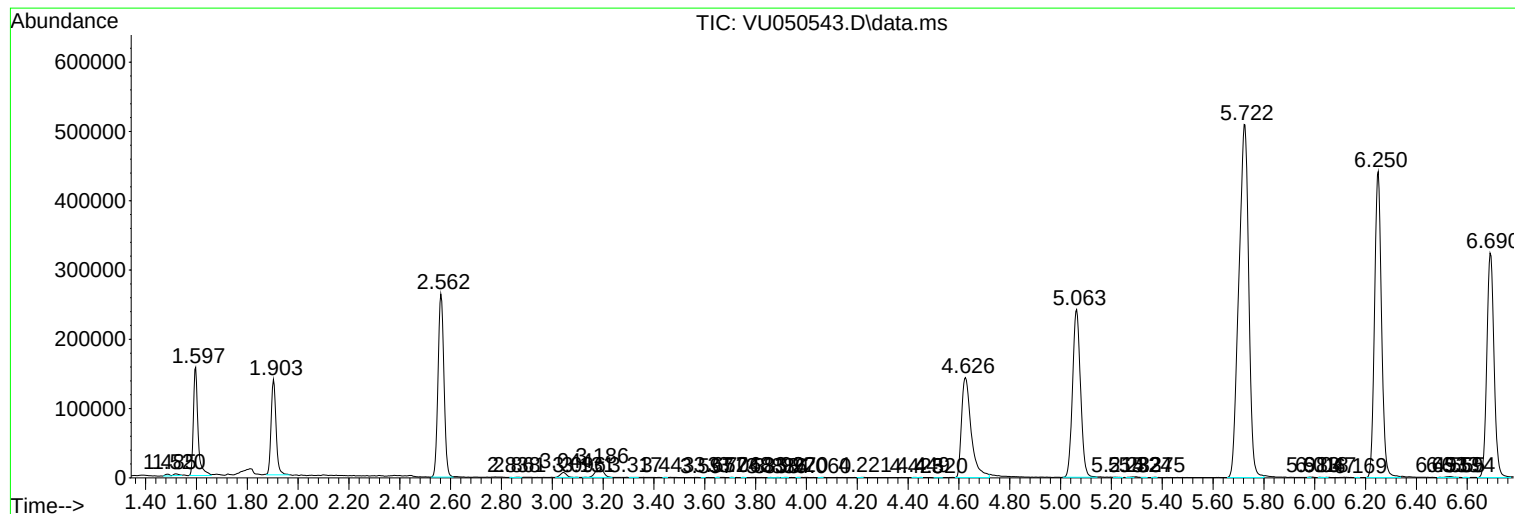

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050543.D
Acq On : 31 Aug 2022 02:24
Operator : SY/MD
Sample : N4345-03ME 100X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050543.D
Acq On : 31 Aug 2022 02:24
Operator : SY/MD
Sample : N4345-03ME 100X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc