

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083023\
 Data File : VU055006.D
 Acq On : 30 Aug 2023 19:22
 Operator : MD/SY
 Sample : 04230-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH493

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.390	25	31	41	rVB	18866	22678	3.00%	0.428%
2	1.595	87	95	102	rBV	26175	31327	4.14%	0.591%
3	1.907	184	192	206	rVB	40106	53165	7.03%	1.003%
4	2.563	382	396	410	rBV3	67731	121962	16.13%	2.300%
5	4.631	1025	1039	1070	rBV2	111368	415539	54.94%	7.838%
6	5.065	1157	1174	1201	rVB4	103843	286911	37.93%	5.412%
7	5.724	1359	1379	1402	rBV2	177122	478737	63.30%	9.030%
8	6.248	1527	1542	1567	rBV	210944	414232	54.77%	7.813%
9	6.541	1620	1633	1650	rBV2	119298	230995	30.54%	4.357%
10	6.688	1666	1679	1699	rBV3	126615	253286	33.49%	4.778%
11	7.566	1938	1952	1968	rBV	49206	90143	11.92%	1.700%
12	7.897	2042	2055	2072	rBV	202372	364787	48.23%	6.881%
13	8.180	2131	2143	2157	rBV3	28878	53189	7.03%	1.003%
14	8.634	2270	2284	2321	rBV3	357403	756340	100.00%	14.266%
15	9.415	2515	2527	2553	rBV	303394	520325	68.80%	9.814%
16	10.756	2930	2944	2960	rBV	119160	196046	25.92%	3.698%
17	10.894	2975	2987	2997	rBV3	4894	8233	1.09%	0.155%
18	11.810	3260	3272	3289	rBV	322459	527532	69.75%	9.950%
19	12.061	3340	3350	3368	rBV3	17046	34855	4.61%	0.657%
20	12.193	3378	3391	3411	rVB	254173	422337	55.84%	7.966%
21	13.843	3895	3904	3920	rBV6	10787	19011	2.51%	0.359%




Sum of corrected areas: 5301630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083023\
Data File : VU055006.D
Acq On : 30 Aug 2023 19:22
Operator : MD/SY
Sample : 04230-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH493

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

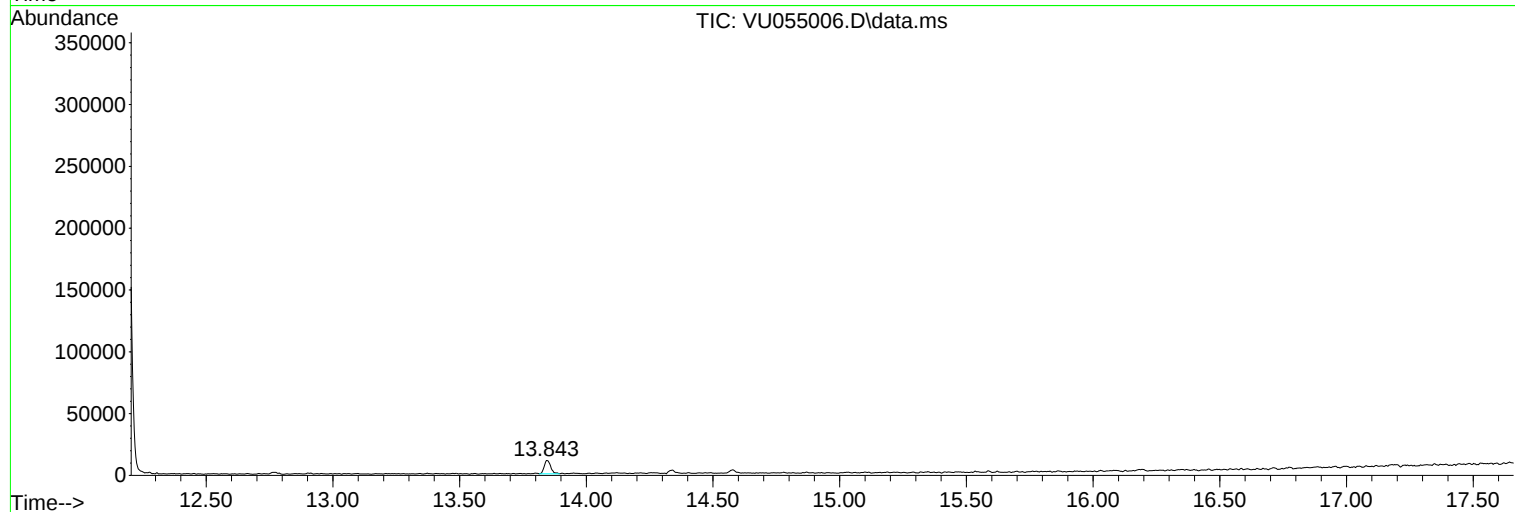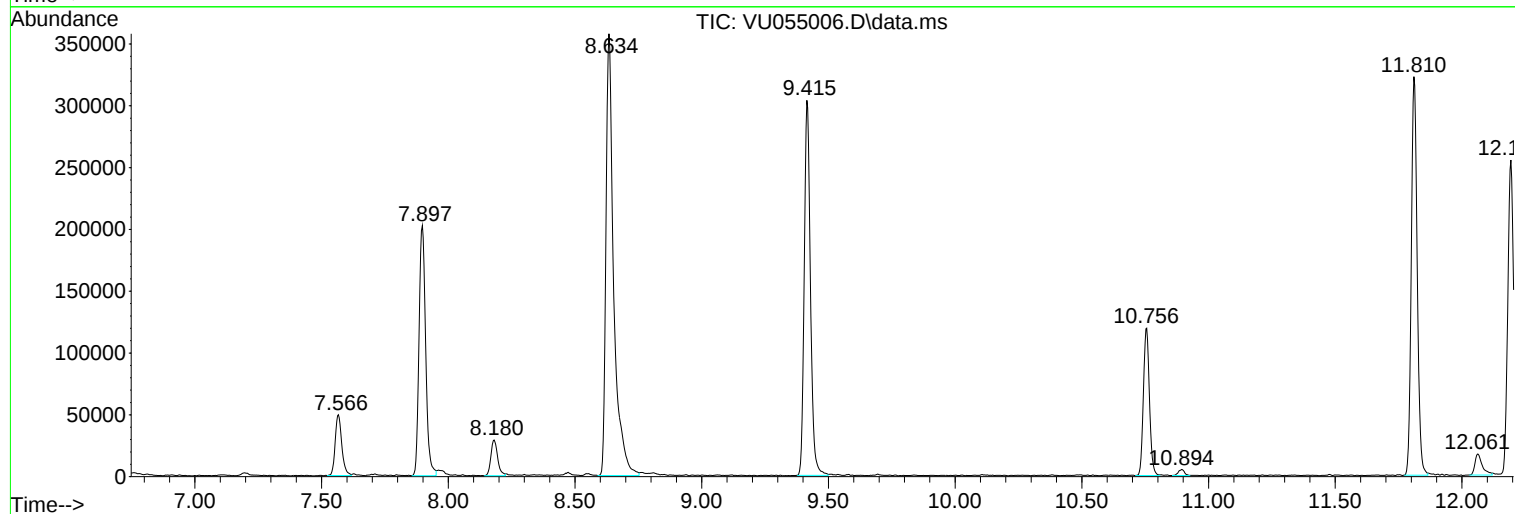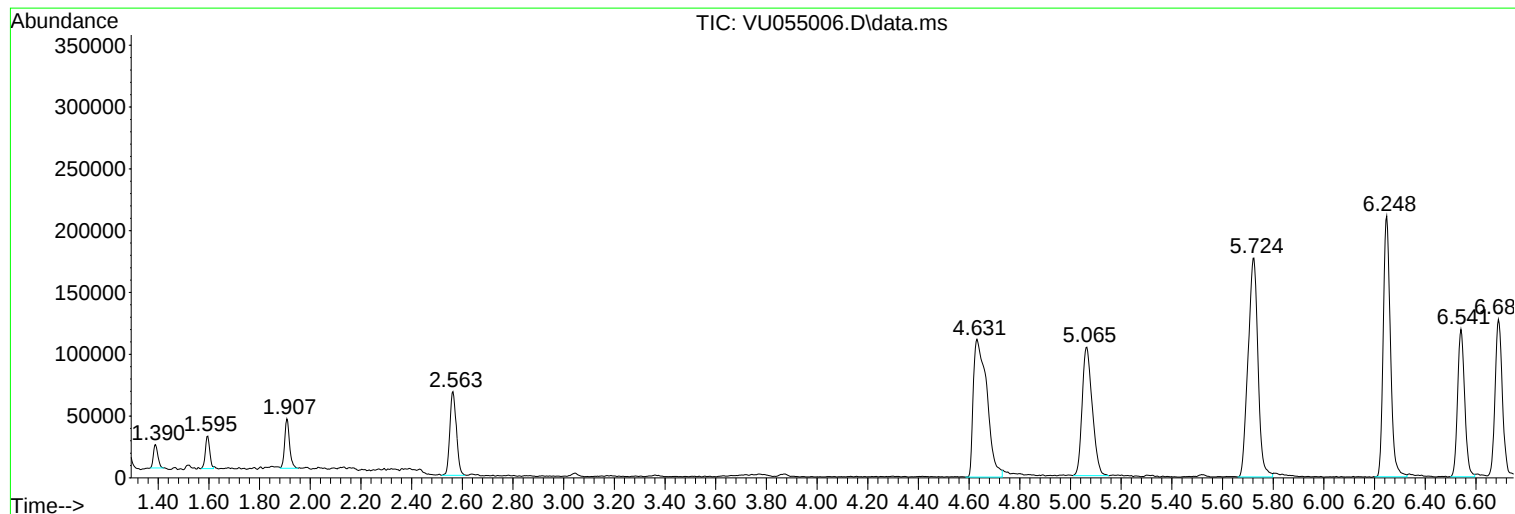

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083023\
Data File : VU055006.D
Acq On : 30 Aug 2023 19:22
Operator : MD/SY
Sample : 04230-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH493

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083023\
Data File : VU055006.D
Acq On : 30 Aug 2023 19:22
Operator : MD/SY
Sample : 04230-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH493

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc