

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU083023\  
 Data File : VU055009.D  
 Acq On : 30 Aug 2023 20:35  
 Operator : MD/SY  
 Sample : VIBLK126  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VIBLK126

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055009.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.039       | 531           | 544         | 563          | rBV      | 96061          | 179089        | 24.16%          | 4.969%        |
| 2         | 3.181       | 573           | 588         | 602          | rBV2     | 16792          | 39655         | 5.35%           | 1.100%        |
| 3         | 4.631       | 1020          | 1039        | 1077         | rBV2     | 153708         | 467334        | 63.06%          | 12.967%       |
| 4         | 5.065       | 1161          | 1174        | 1191         | rVB4     | 15217          | 38760         | 5.23%           | 1.075%        |
| 5         | 5.708       | 1362          | 1374        | 1392         | rBV3     | 14125          | 36063         | 4.87%           | 1.001%        |
| 6         | 6.248       | 1529          | 1542        | 1562         | rBV      | 231041         | 450567        | 60.79%          | 12.502%       |
| 7         | 6.541       | 1619          | 1633        | 1654         | rBV3     | 48213          | 96275         | 12.99%          | 2.671%        |
| 8         | 6.692       | 1666          | 1680        | 1692         | rBV4     | 14825          | 30192         | 4.07%           | 0.838%        |
| 9         | 7.570       | 1944          | 1953        | 1964         | rBV4     | 5048           | 8631          | 1.16%           | 0.239%        |
| 10        | 8.184       | 2135          | 2144        | 2154         | rBV3     | 5003           | 7605          | 1.03%           | 0.211%        |
| 11        | 8.634       | 2272          | 2284        | 2317         | rBV3     | 343396         | 741126        | 100.00%         | 20.563%       |
| 12        | 9.415       | 2515          | 2527        | 2553         | rBV      | 349653         | 597210        | 80.58%          | 16.570%       |
| 13        | 10.756      | 2932          | 2944        | 2963         | rBV2     | 94407          | 154372        | 20.83%          | 4.283%        |
| 14        | 11.811      | 3259          | 3272        | 3294         | rBV      | 377733         | 622601        | 84.01%          | 17.275%       |
| 15        | 12.193      | 3380          | 3391        | 3409         | rBV2     | 75148          | 125545        | 16.94%          | 3.483%        |
| 16        | 13.846      | 3896          | 3905        | 3923         | rBV8     | 4863           | 9063          | 1.22%           | 0.251%        |




Sum of corrected areas: 3604088

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU083023\  
Data File : VU055009.D  
Acq On : 30 Aug 2023 20:35  
Operator : MD/SY  
Sample : VIBLK126  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR082823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

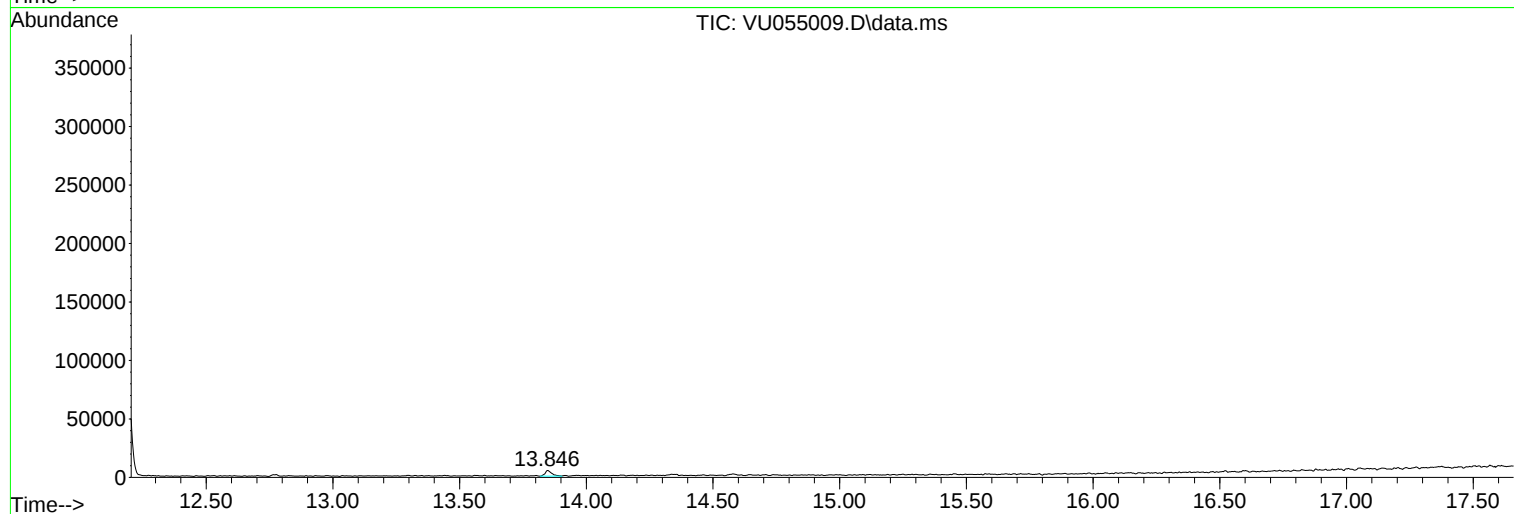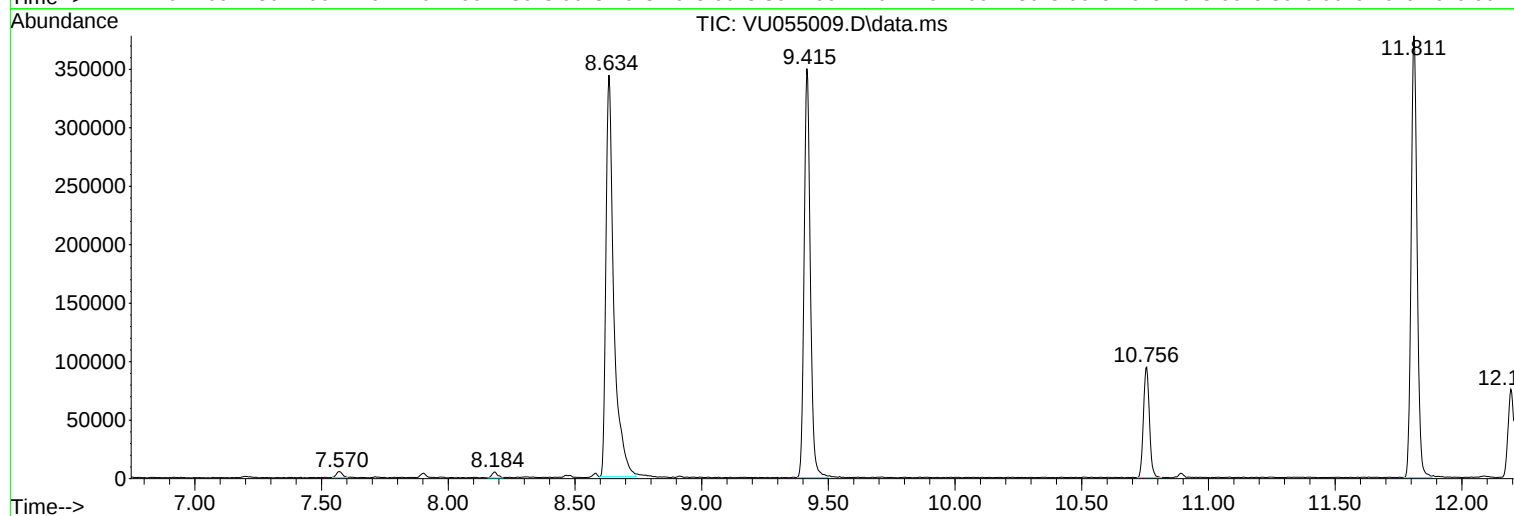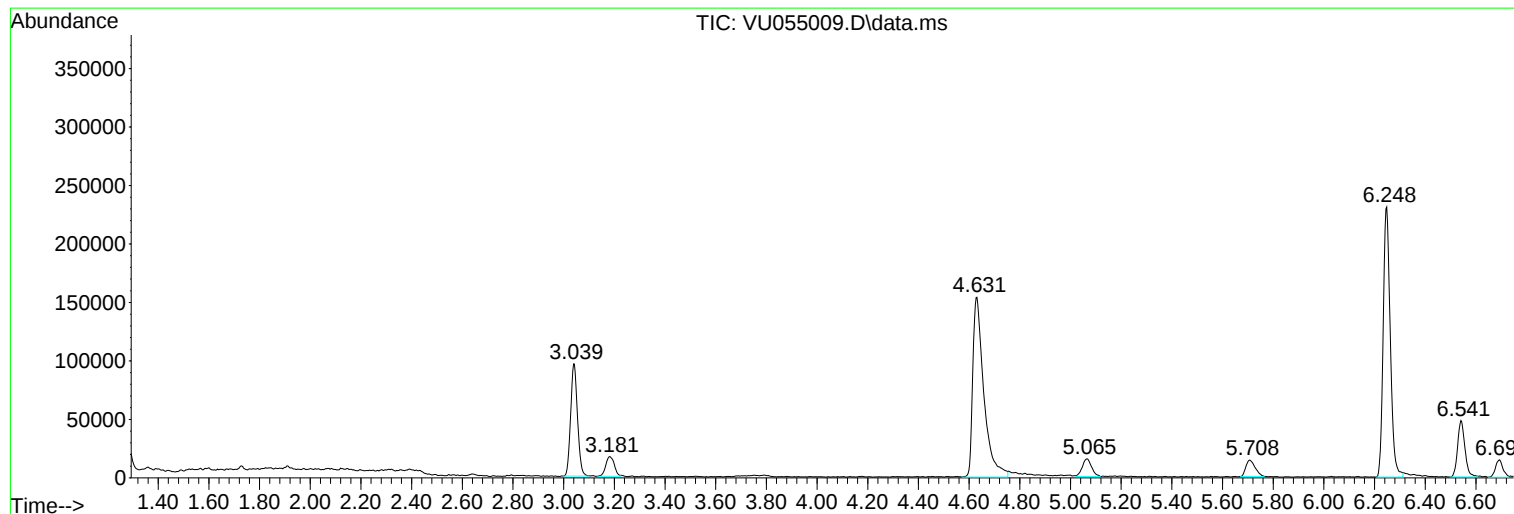

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU083023\  
Data File : VU055009.D  
Acq On : 30 Aug 2023 20:35  
Operator : MD/SY  
Sample : VIBLK126  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR082823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU083023\  
Data File : VU055009.D  
Acq On : 30 Aug 2023 20:35  
Operator : MD/SY  
Sample : VIBLK126  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR082823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |