


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083023\
Data File : VU054988.D
Acq On : 30 Aug 2023 09:18
Operator : MD/SY
Sample : BFB036
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB036

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 01 04:57:47 2023

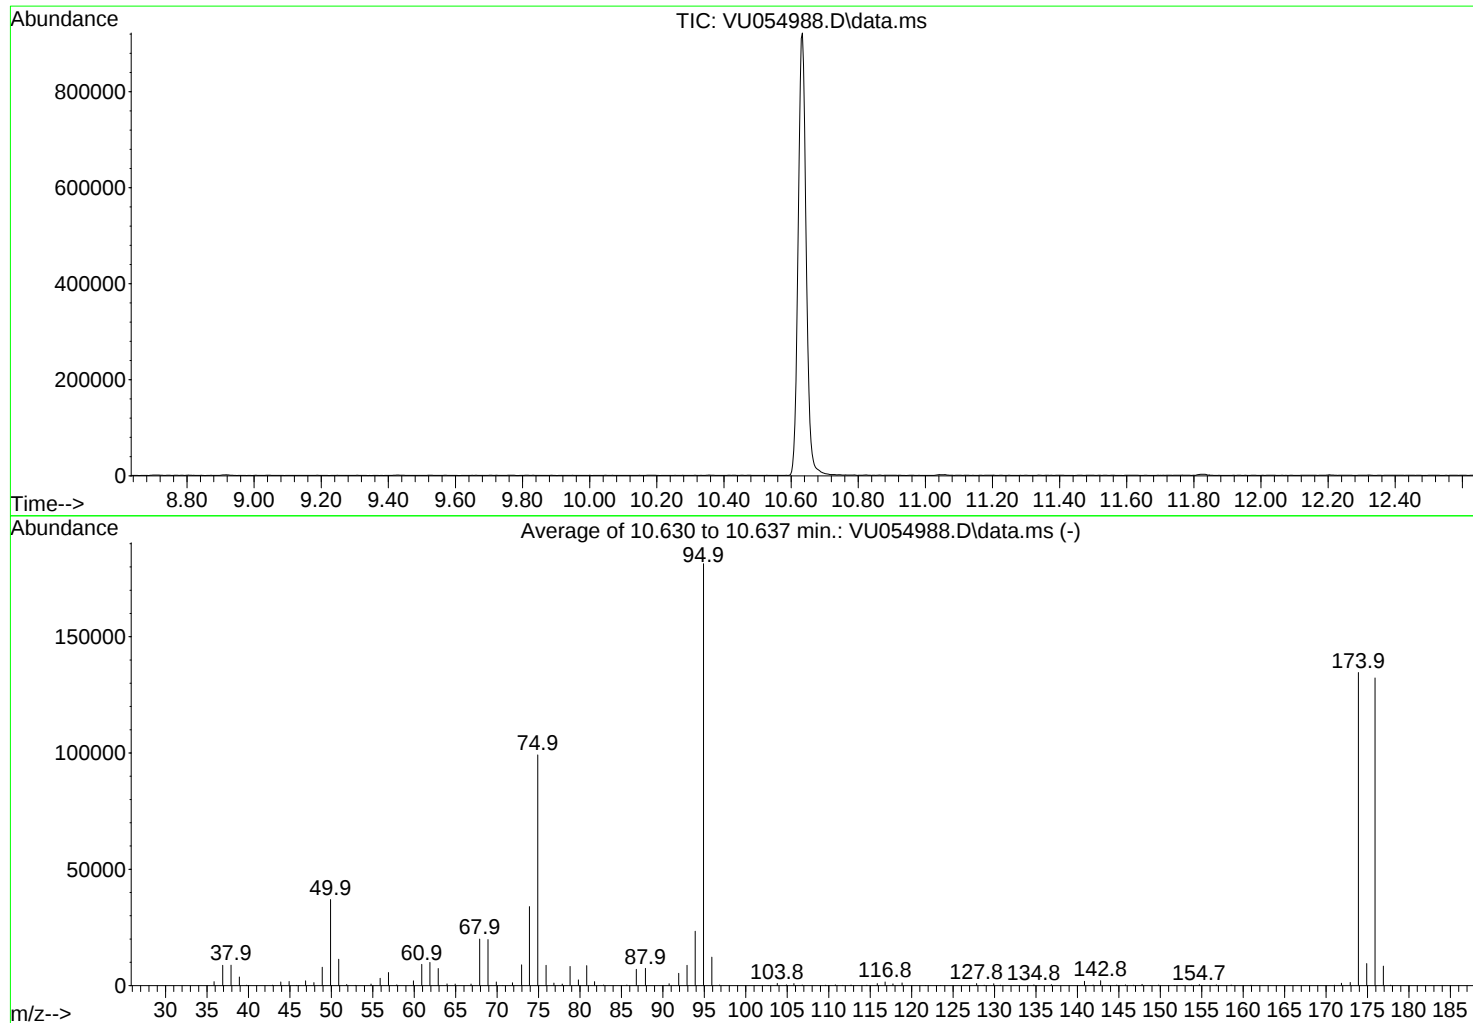

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	37021	PASS
75	95	30	80	54.7	99189	PASS
95	95	100	100	100.0	181376	PASS
96	95	5	9	6.7	12218	PASS
173	174	0.00	2	1.0	1356	PASS
174	95	50	120	74.2	134592	PASS
175	174	5	9	7.1	9500	PASS
176	174	95	101	98.3	132259	PASS
177	176	5	9	6.3	8348	PASS

m/z	Abundance
39.80	209.0
43.90	752.0
55.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.80	1823.0
36.90	9037.0
37.90	8999.0
38.90	3693.0
39.80	387.0
43.00	122.0
43.90	2504.0
44.90	1900.0
45.80	143.0
46.90	2102.0
47.90	1328.0
48.90	7935.0
49.90	38592.0
50.90	11396.0
51.90	499.0
52.90	137.0
54.80	721.0
55.90	3316.0
56.90	5668.0
57.90	277.0
59.90	2034.0
60.90	9397.0
61.90	10326.0
62.90	7483.0
64.00	707.0
65.00	759.0
66.80	606.0
67.90	20504.0
68.90	20760.0
69.90	1655.0
71.90	1466.0
73.00	9031.0
73.90	35272.0
74.90	101832.0
75.90	8834.0
76.90	1021.0
77.90	710.0
78.80	8558.0
79.80	2612.0
80.80	8621.0
81.80	1768.0
82.80	213.0
85.60	281.0
86.80	7556.0
87.90	7384.0
90.70	878.0
91.90	5287.0
92.90	8774.0
93.90	23536.0
94.90	185664.0
95.90	12376.0
96.90	233.0
103.80	930.0
104.90	313.0
105.80	885.0
106.80	350.0
109.70	185.0
110.80	290.0
111.70	145.0
112.70	213.0
114.60	208.0
115.80	937.0
116.80	1483.0
117.80	807.0
118.80	1122.0
121.70	111.0
127.90	894.0
128.70	216.0
129.90	753.0
130.70	150.0
134.80	314.0
136.80	356.0
140.90	1868.0
141.90	275.0
142.80	2204.0
143.80	100.0
144.80	220.0
145.80	245.0
146.80	147.0
147.80	474.0
148.80	111.0
149.80	197.0
151.70	116.0
152.80	115.0
153.80	137.0
154.70	463.0
156.90	312.0
158.60	300.0
160.90	120.0
171.10	201.0
171.80	985.0
172.90	1423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

173.90	133440.0
174.90	9776.0
175.90	131712.0
176.90	8173.0
177.80	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.80	1721.0
36.90	8881.0
37.90	9147.0
38.90	3785.0
39.80	412.0
42.90	146.0
43.90	2390.0
44.90	1831.0
45.80	173.0
46.90	2082.0
47.90	1297.0
48.90	8188.0
49.90	38152.0
50.90	11637.0
51.80	466.0
52.90	108.0
54.80	637.0
55.90	3343.0
56.90	5754.0
57.90	357.0
59.90	2088.0
60.90	9375.0
61.90	10229.0
62.90	7485.0
63.90	749.0
65.00	686.0
66.90	689.0
67.90	20456.0
68.90	20320.0
69.90	1565.0
71.90	1227.0
72.90	9327.0
73.90	34728.0
74.90	101968.0
75.90	9118.0
76.90	1099.0
77.80	634.0
78.80	8418.0
79.80	2482.0
80.80	8815.0
81.80	1798.0
82.80	228.0
85.70	207.0
86.80	7089.0
87.90	7692.0
90.70	821.0
91.90	5387.0
92.90	8920.0
93.90	24160.0
94.90	187072.0
95.90	12483.0
96.80	235.0
103.80	958.0
104.90	337.0
105.80	859.0
106.80	272.0
109.60	173.0
110.80	305.0
111.70	104.0
112.70	271.0
114.60	214.0
115.90	917.0
116.80	1598.0
117.80	783.0
118.90	1156.0
127.80	895.0
128.80	204.0
129.90	851.0
130.70	179.0
134.70	333.0
136.80	391.0
140.90	1867.0
141.90	296.0
142.80	2149.0
143.80	155.0
144.80	248.0
145.80	379.0
146.80	168.0
147.80	606.0
149.80	228.0
153.70	171.0
154.70	477.0
156.70	316.0
158.60	285.0
161.00	162.0
171.00	174.0
171.90	1057.0
172.90	1401.0
173.90	138688.0
174.90	9794.0
175.90	136064.0
176.90	8605.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

177.80

208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	1549.0
36.90	8199.0
37.90	8148.0
38.90	3520.0
39.80	378.0
42.80	164.0
43.90	2133.0
44.90	1549.0
46.10	197.0
46.90	1965.0
47.90	1121.0
48.90	7587.0
49.90	34320.0
50.90	10863.0
51.80	351.0
54.80	540.0
55.90	2985.0
56.90	5322.0
57.90	364.0
59.90	1910.0
60.90	8681.0
61.90	9214.0
62.90	6987.0
63.90	689.0
64.90	565.0
66.90	592.0
67.90	19032.0
68.90	18232.0
69.90	1444.0
70.70	133.0
71.80	944.0
72.90	8427.0
73.90	31920.0
74.90	93768.0
75.90	8260.0
76.80	1141.0
77.90	546.0
78.80	7683.0
79.80	2216.0
80.80	8323.0
81.70	1558.0
82.90	319.0
85.70	164.0
86.80	6375.0
87.90	7042.0
90.80	762.0
91.90	5103.0
92.90	8362.0
93.90	22368.0
94.90	171392.0
95.90	11794.0
96.90	233.0
102.70	104.0
103.80	900.0
104.90	357.0
105.80	837.0
106.80	168.0
109.70	147.0
110.80	292.0
112.70	259.0
114.60	181.0
115.90	780.0
116.80	1510.0
117.70	685.0
118.80	1079.0
123.50	101.0
127.80	755.0
128.80	212.0
129.90	783.0
130.70	188.0
134.70	349.0
136.90	377.0
140.80	1777.0
141.90	262.0
142.80	1967.0
143.80	155.0
144.70	234.0
145.80	417.0
146.80	154.0
147.80	596.0
149.80	253.0
153.70	156.0
154.70	493.0
156.70	296.0
158.50	223.0
161.00	218.0
170.90	181.0
171.90	1001.0
172.90	1245.0
173.90	131648.0
174.90	8931.0
175.90	129000.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

176.908266.0

177.80193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036