

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060573.D
 Acq On : 30 Aug 2024 15:20
 Operator : MD/SY
 Sample : P3768-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 01:02:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5396	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	8106	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2338	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3616	0.412	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	82.000%
4) 1,2-Dichloroethane-d4	5.685	65	2155	0.463	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
7) 1,2-Dichloropropane-d6	6.687	67	2442	0.485	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	96.000%
8) Toluene-d8	7.888	98	5612	0.539	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1973	0.447	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	90.000%
Target Compounds						
12) 1,2,3-Trichloropropane	10.865	75	56	0.021	ug/L #	76
13) 1,2-Dibromo-3-chloropr...	12.751	75	61	0.116	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060573.D
Acq On : 30 Aug 2024 15:20
Operator : MD/SY
Sample : P3768-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 31 01:02:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

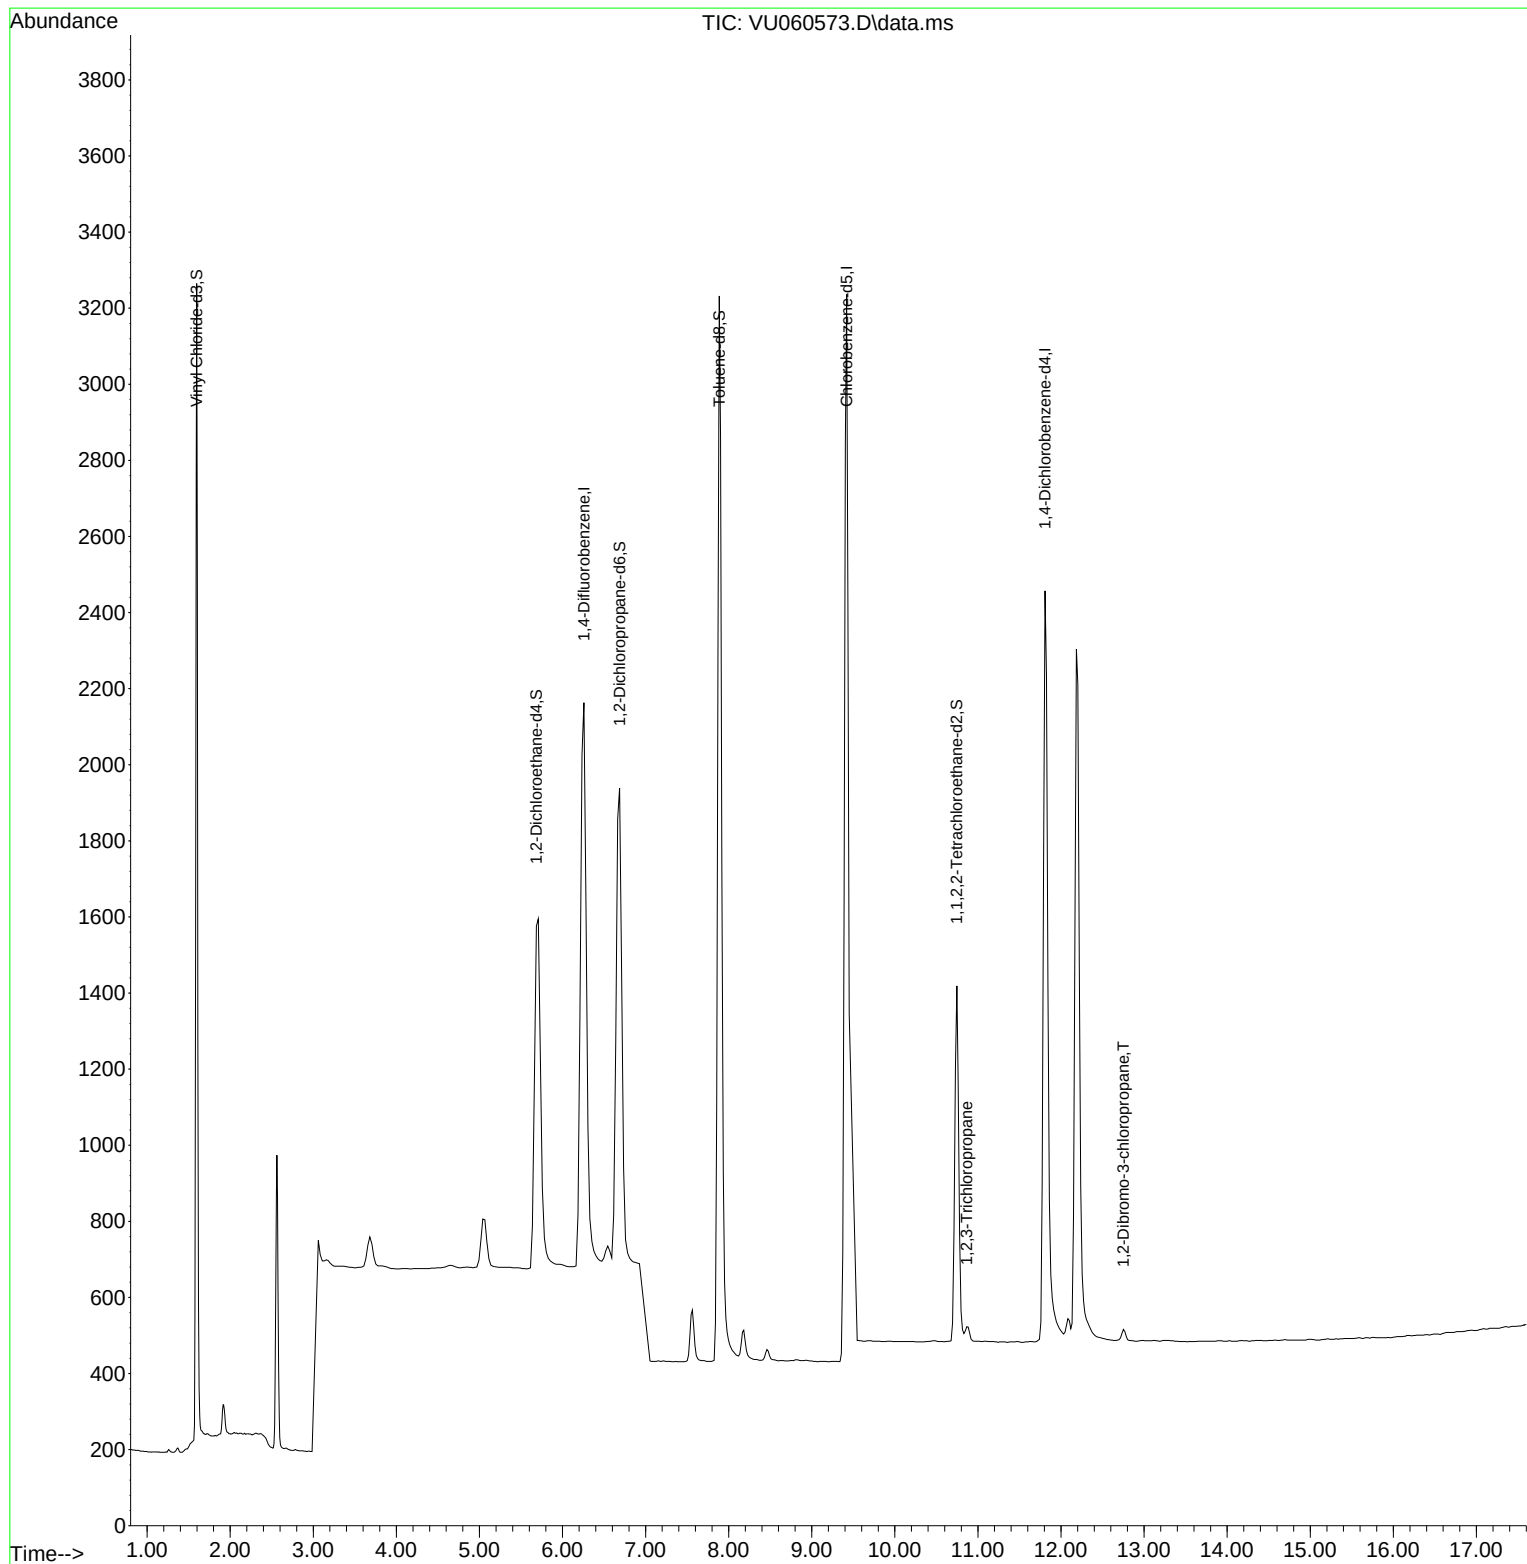

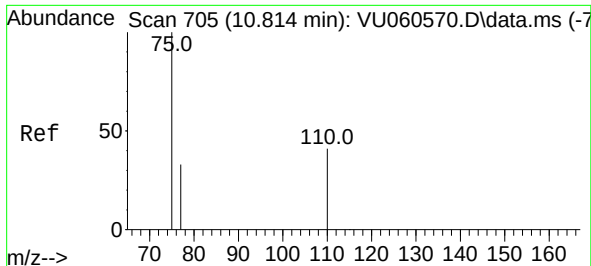

#12

1,2,3-Trichloropropane

Concen: 0.021 ug/L

RT: 10.865 min Scan# 705

Delta R.T. 0.052 min

Lab File: VU060573.D





Acq: 30 Aug 2024 15:20

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion:	75	Resp:	56
Ion	Ratio	Lower	Upper
75	100		
110	42.9	32.4	48.6
77	5.4	26.0	39.0

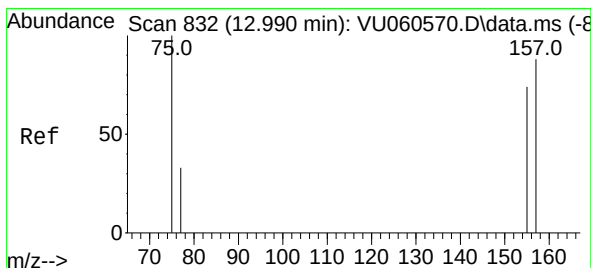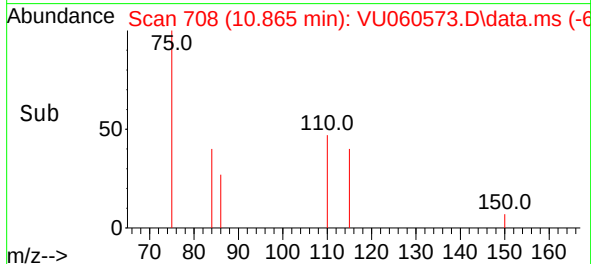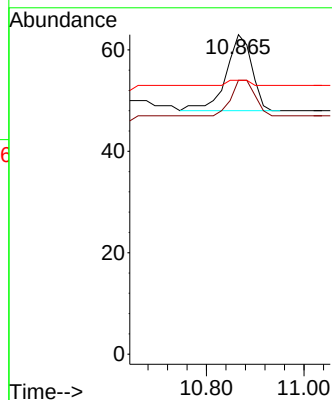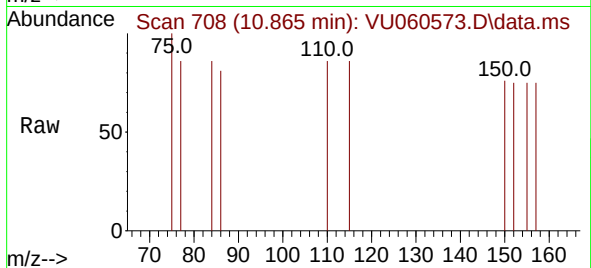

#13

1,2-Dibromo-3-chloropropane

Concen: 0.116 ug/L

RT: 12.751 min Scan# 818

Delta R.T. -0.240 min

Lab File: VU060573.D

Acq: 30 Aug 2024 15:20

Tgt Ion:	75	Resp:	61
Ion	Ratio	Lower	Upper
75	100		
157	66.2	74.3	111.5
155	71.8	66.2	99.2

