

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060575.D
 Acq On : 30 Aug 2024 16:07
 Operator : MD/SY
 Sample : P3768-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 01:02:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5278	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	8128	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2384	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3815	0.444	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.709	65	2278	0.501	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2540	0.503	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	100.000%		
8) Toluene-d8	7.887	98	5863	0.562	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	112.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2070	0.468	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	94.000%		
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.990	75	68	0.127	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060575.D
Acq On : 30 Aug 2024 16:07
Operator : MD/SY
Sample : P3768-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Aug 31 01:02:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

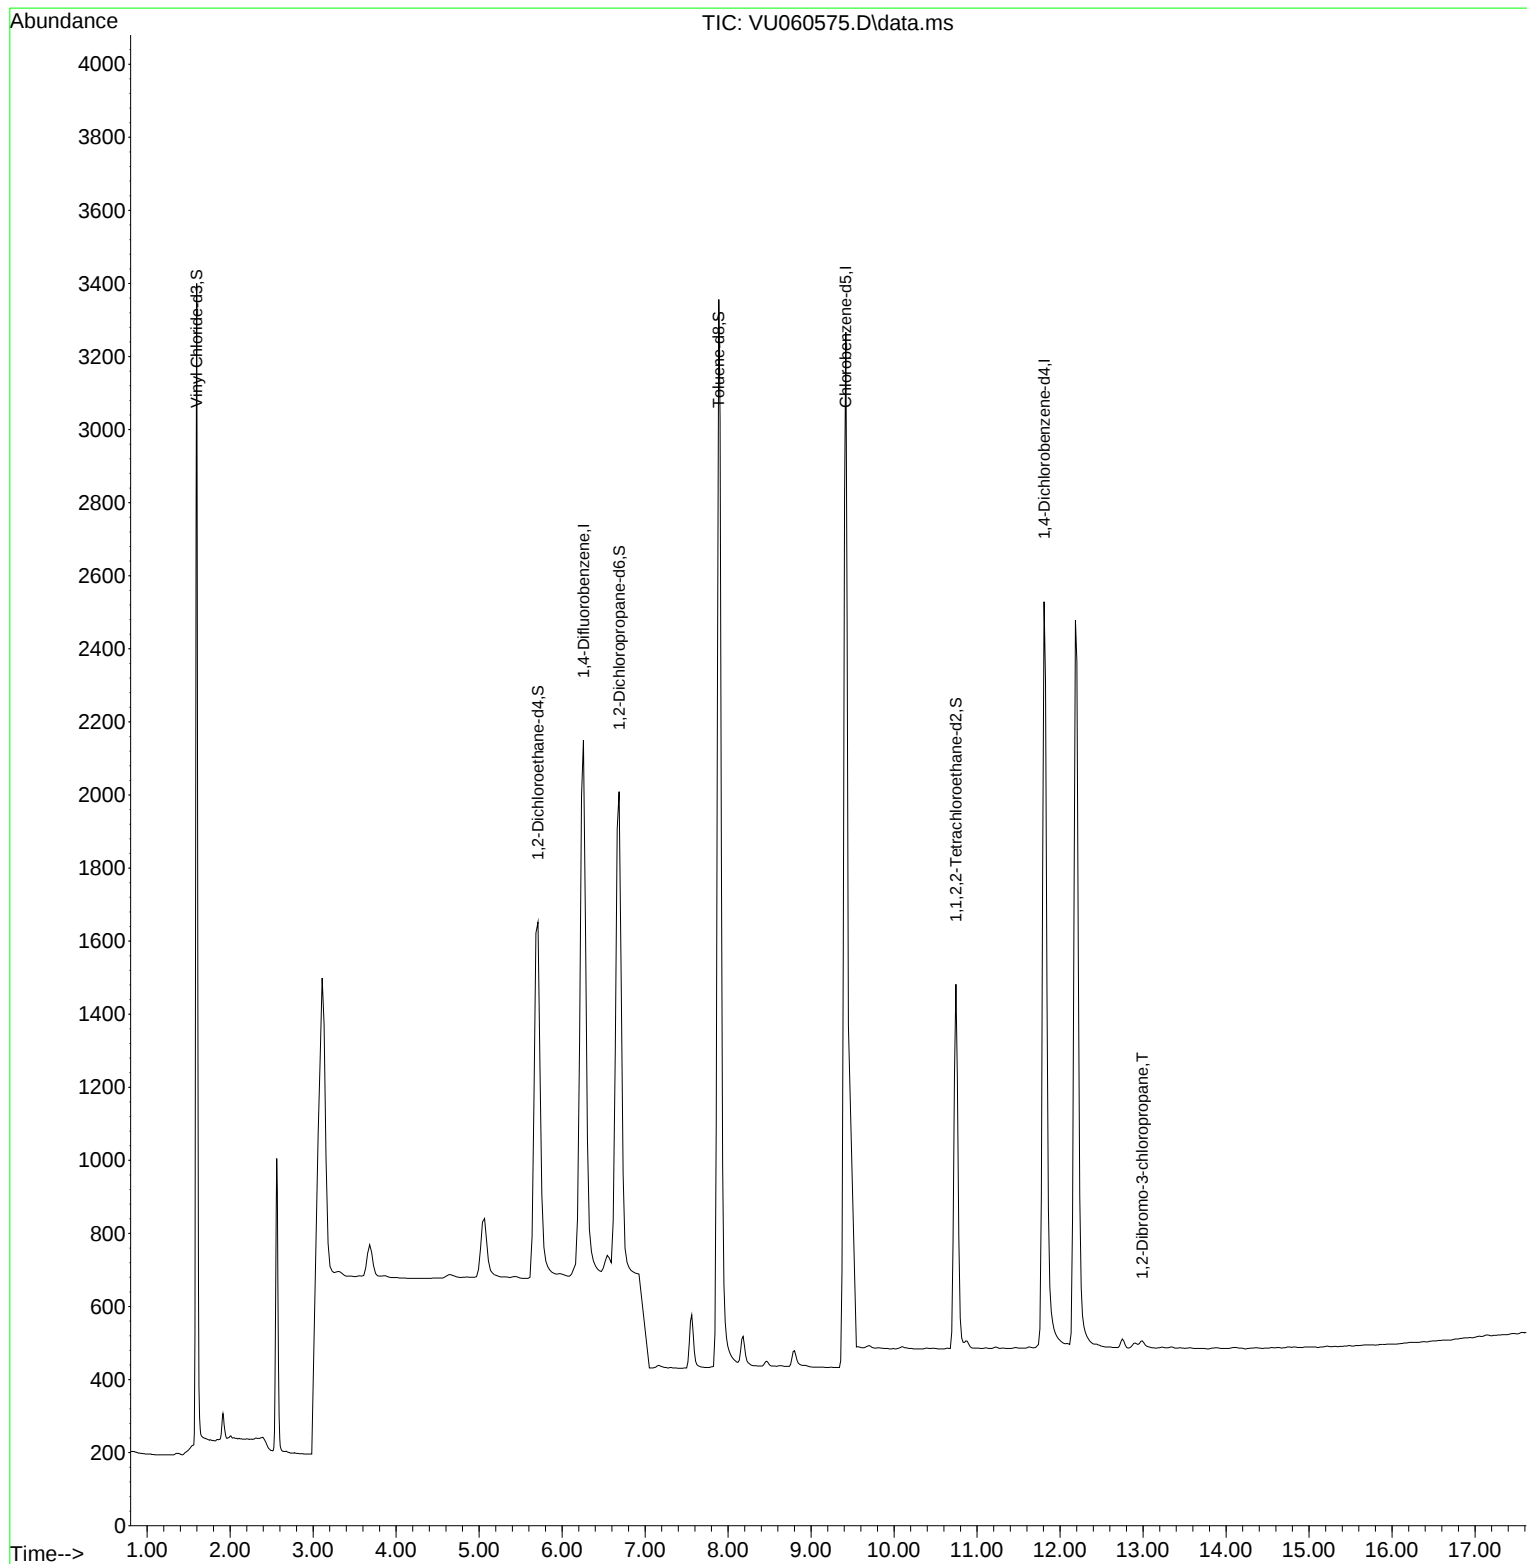

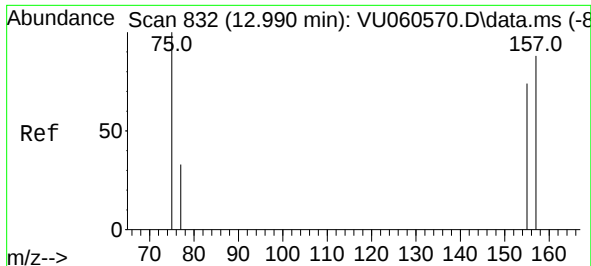

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.127 ug/L
 RT: 12.990 min Scan# 84
 Delta R.T. -0.000 min
 Lab File: VU060575.D
 Acq: 30 Aug 2024 16:07

Instrument :
 MSVOA_U
 ClientSampleId :

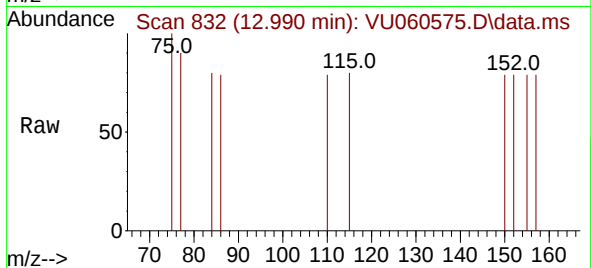

Tgt Ion: 75	Resp:	68
Ion	Ratio	Lower Upper
75	100	
157	78.7	74.3 111.5
155	78.7	66.2 99.2

