

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060578.D
 Acq On : 30 Aug 2024 16:56
 Operator : MD/SY
 Sample : P3803-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 01:02:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5500	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	8908	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3074	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3696	0.413	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	82.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2306	0.486	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3004	0.542	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	108.000%		
8) Toluene-d8	7.887	98	6326	0.553	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	110.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2209	0.455	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	92.000%		
Target Compounds						
					Qvalue	
6) Trichloroethene	6.639	95	235	0.042	ug/L #	61
13) 1,2-Dibromo-3-chloropr...	12.956	75	87	0.126	ug/L #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060578.D
Acq On : 30 Aug 2024 16:56
Operator : MD/SY
Sample : P3803-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Aug 31 01:02:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

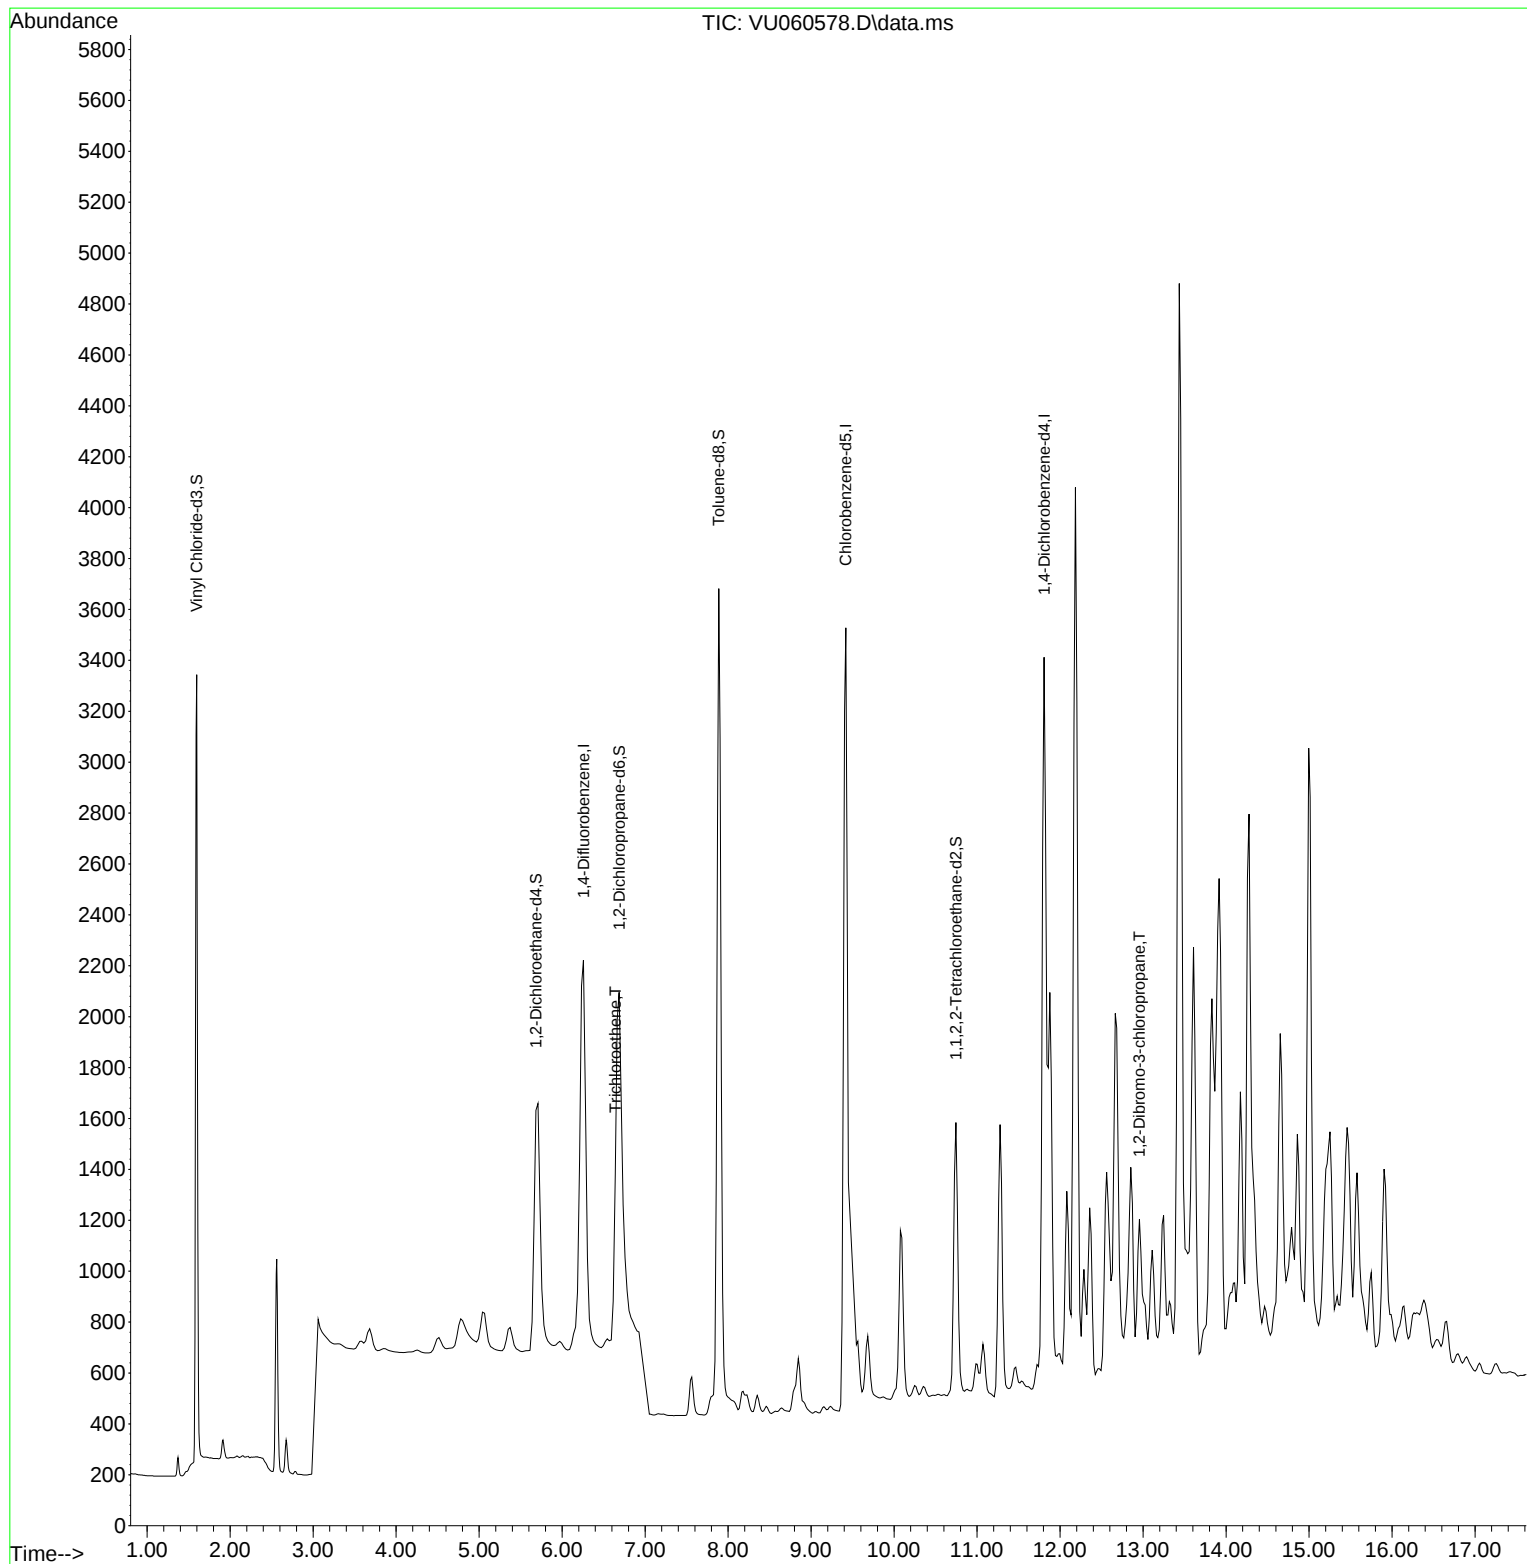

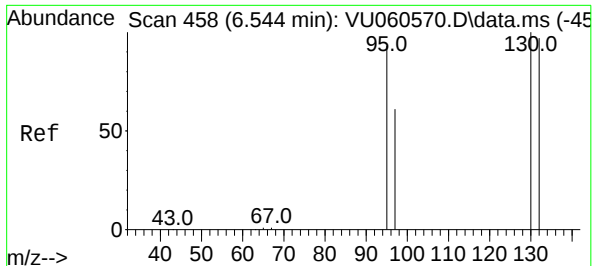




#6
Trichloroethene
Concen: 0.042 ug/L
RT: 6.639 min Scan# 41
Delta R.T. 0.095 min
Lab File: VU060578.D
Acq: 30 Aug 2024 16:56

Instrument :
MSVOA_U
ClientSampleId :

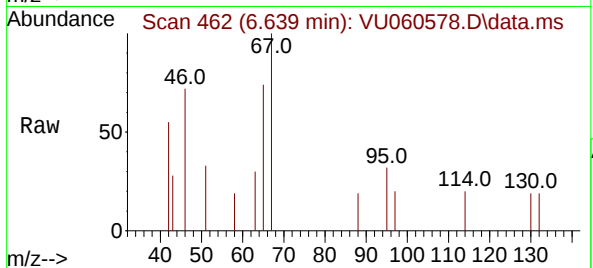

Tgt Ion: 95 Resp: 235

Ion	Ratio	Lower	Upper
95	100		
97	61.0	48.5	90.1
132	57.3	75.5	140.1#
130	58.5	76.3	141.7#

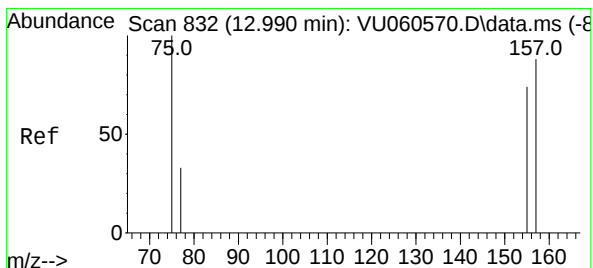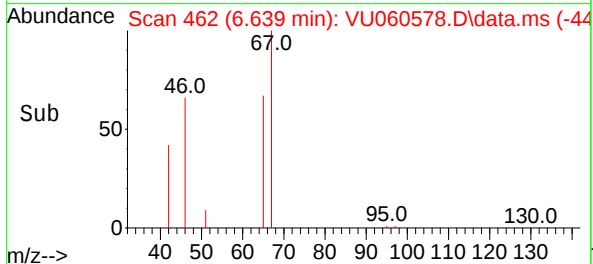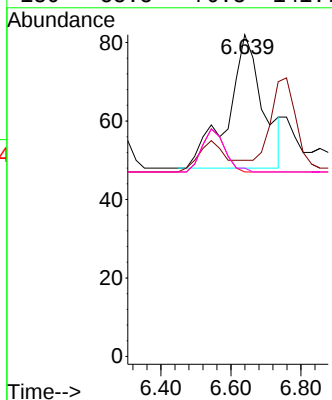

#13
1,2-Dibromo-3-chloropropane
Concen: 0.126 ug/L
RT: 12.956 min Scan# 830
Delta R.T. -0.034 min
Lab File: VU060578.D
Acq: 30 Aug 2024 16:56

Tgt Ion: 75 Resp: 87

Ion	Ratio	Lower	Upper
75	100		
157	62.3	74.3	111.5#
155	62.3	66.2	99.2#

