

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060579.D
 Acq On : 30 Aug 2024 17:45
 Operator : MD/SY
 Sample : VIBLK006
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 05 17:42:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5637	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	8369	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2439	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3708	0.404	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	80.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2315	0.476	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2566	0.493	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	98.000%		
8) Toluene-d8	7.887	98	6084	0.566	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	114.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2021	0.443	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.750	75	21	0.038	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060579.D
Acq On : 30 Aug 2024 17:45
Operator : MD/SY
Sample : VIBLK006
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Sep 05 17:42:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

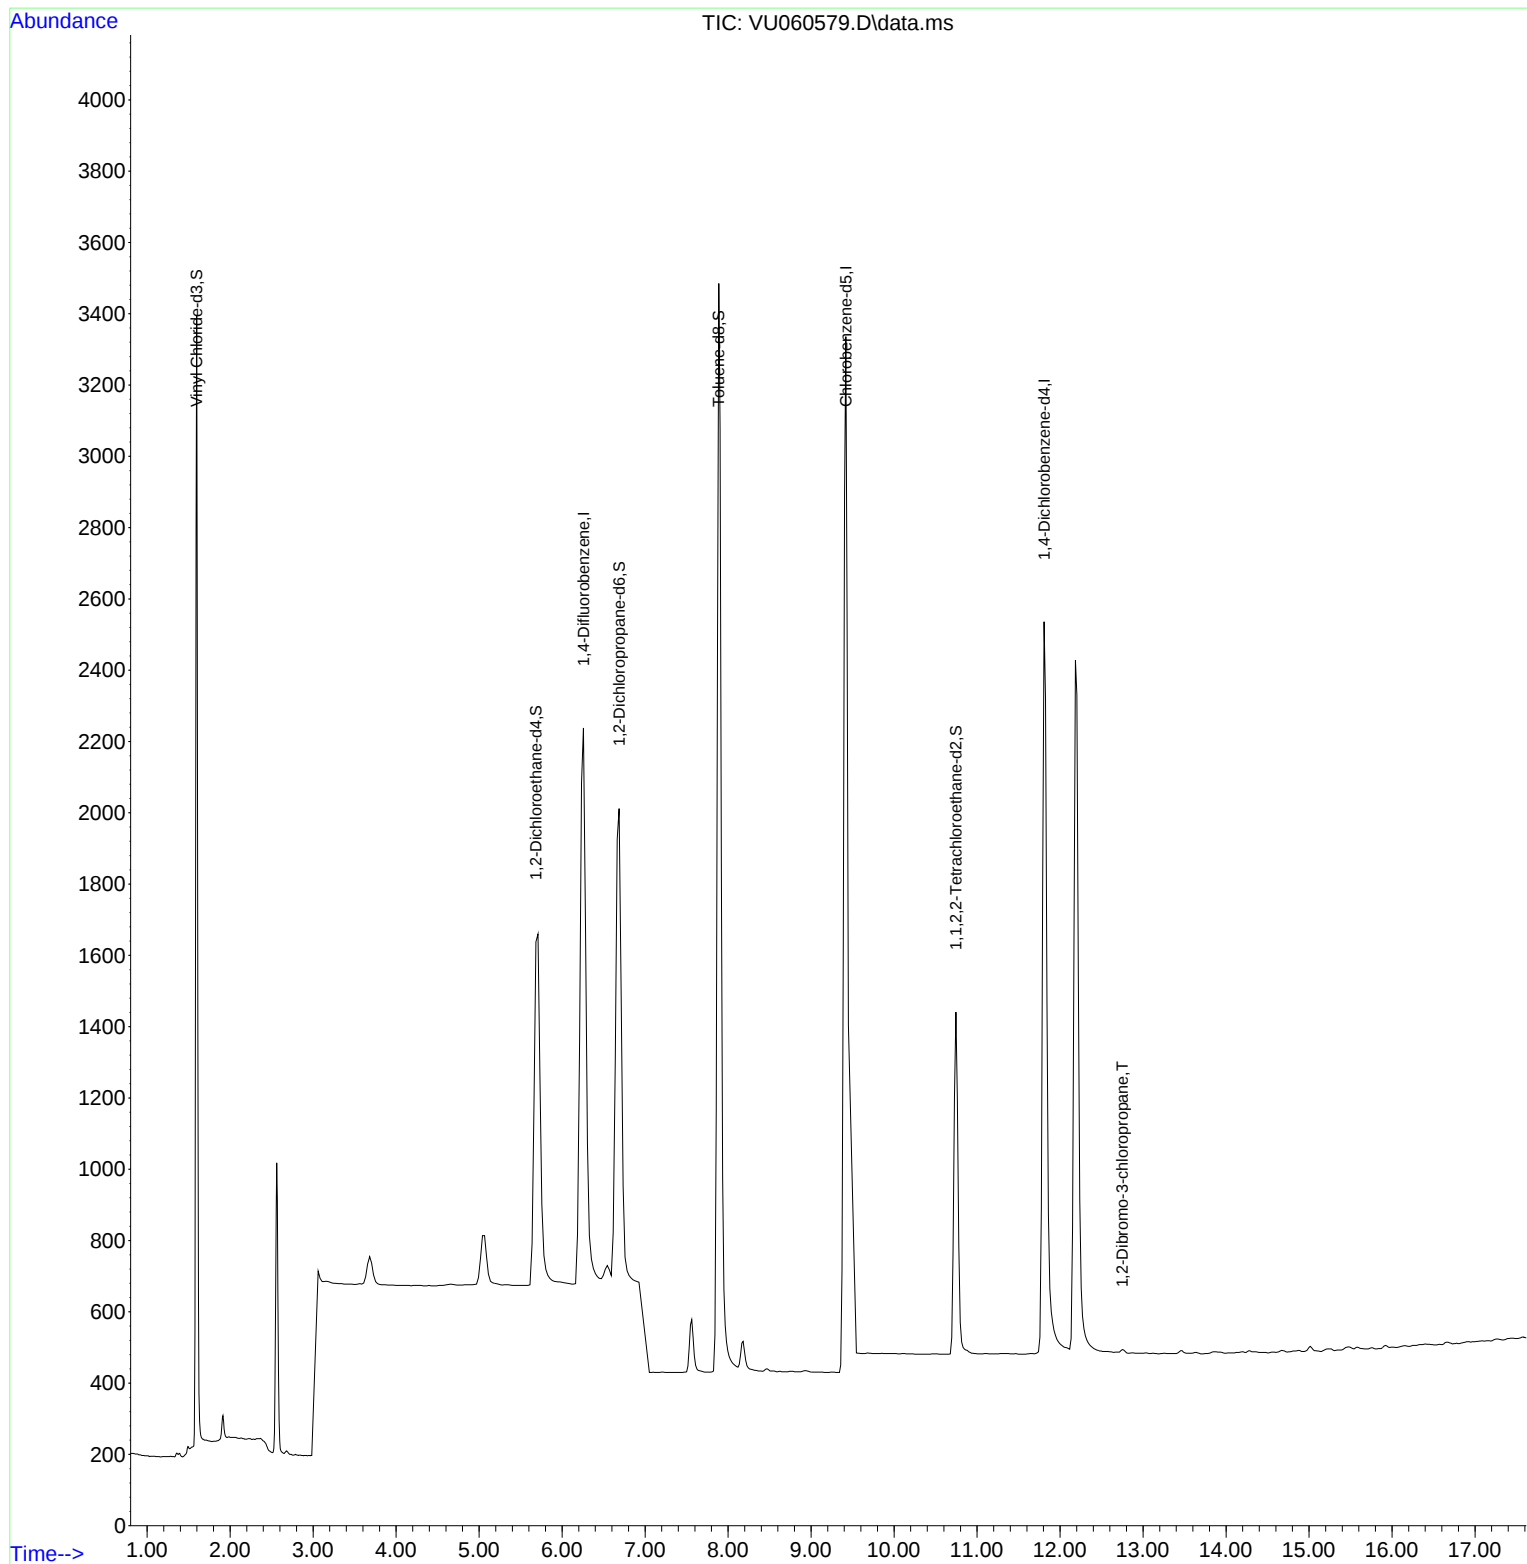

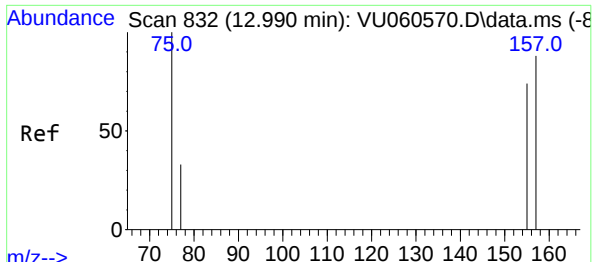

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.038 ug/L
 RT: 12.750 min Scan# 81
 Delta R.T. -0.240 min
 Lab File: VU060579.D
 Acq: 30 Aug 2024 17:45

Instrument :
 MSVOA_U
 ClientSampleId :

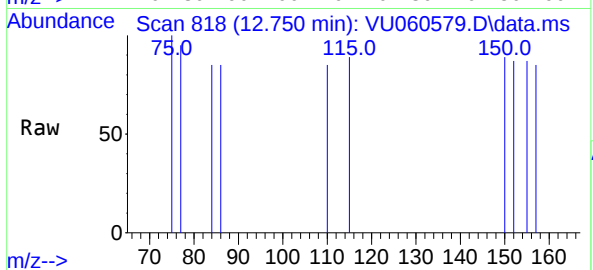

Tgt Ion: 75	Resp: 21
Ion Ratio	Lower Upper
75 100	
157 85.5	74.3 111.5
155 87.3	66.2 99.2

