

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060581.D
 Acq On : 30 Aug 2024 18:09
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 01:03:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5264	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	8017	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2283	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3511	0.410	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	82.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2186	0.482	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2424	0.486	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	98.000%		
8) Toluene-d8	7.887	98	5646	0.548	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	110.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1932	0.443	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.750	75	20	0.039	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060581.D
Acq On : 30 Aug 2024 18:09
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Aug 31 01:03:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

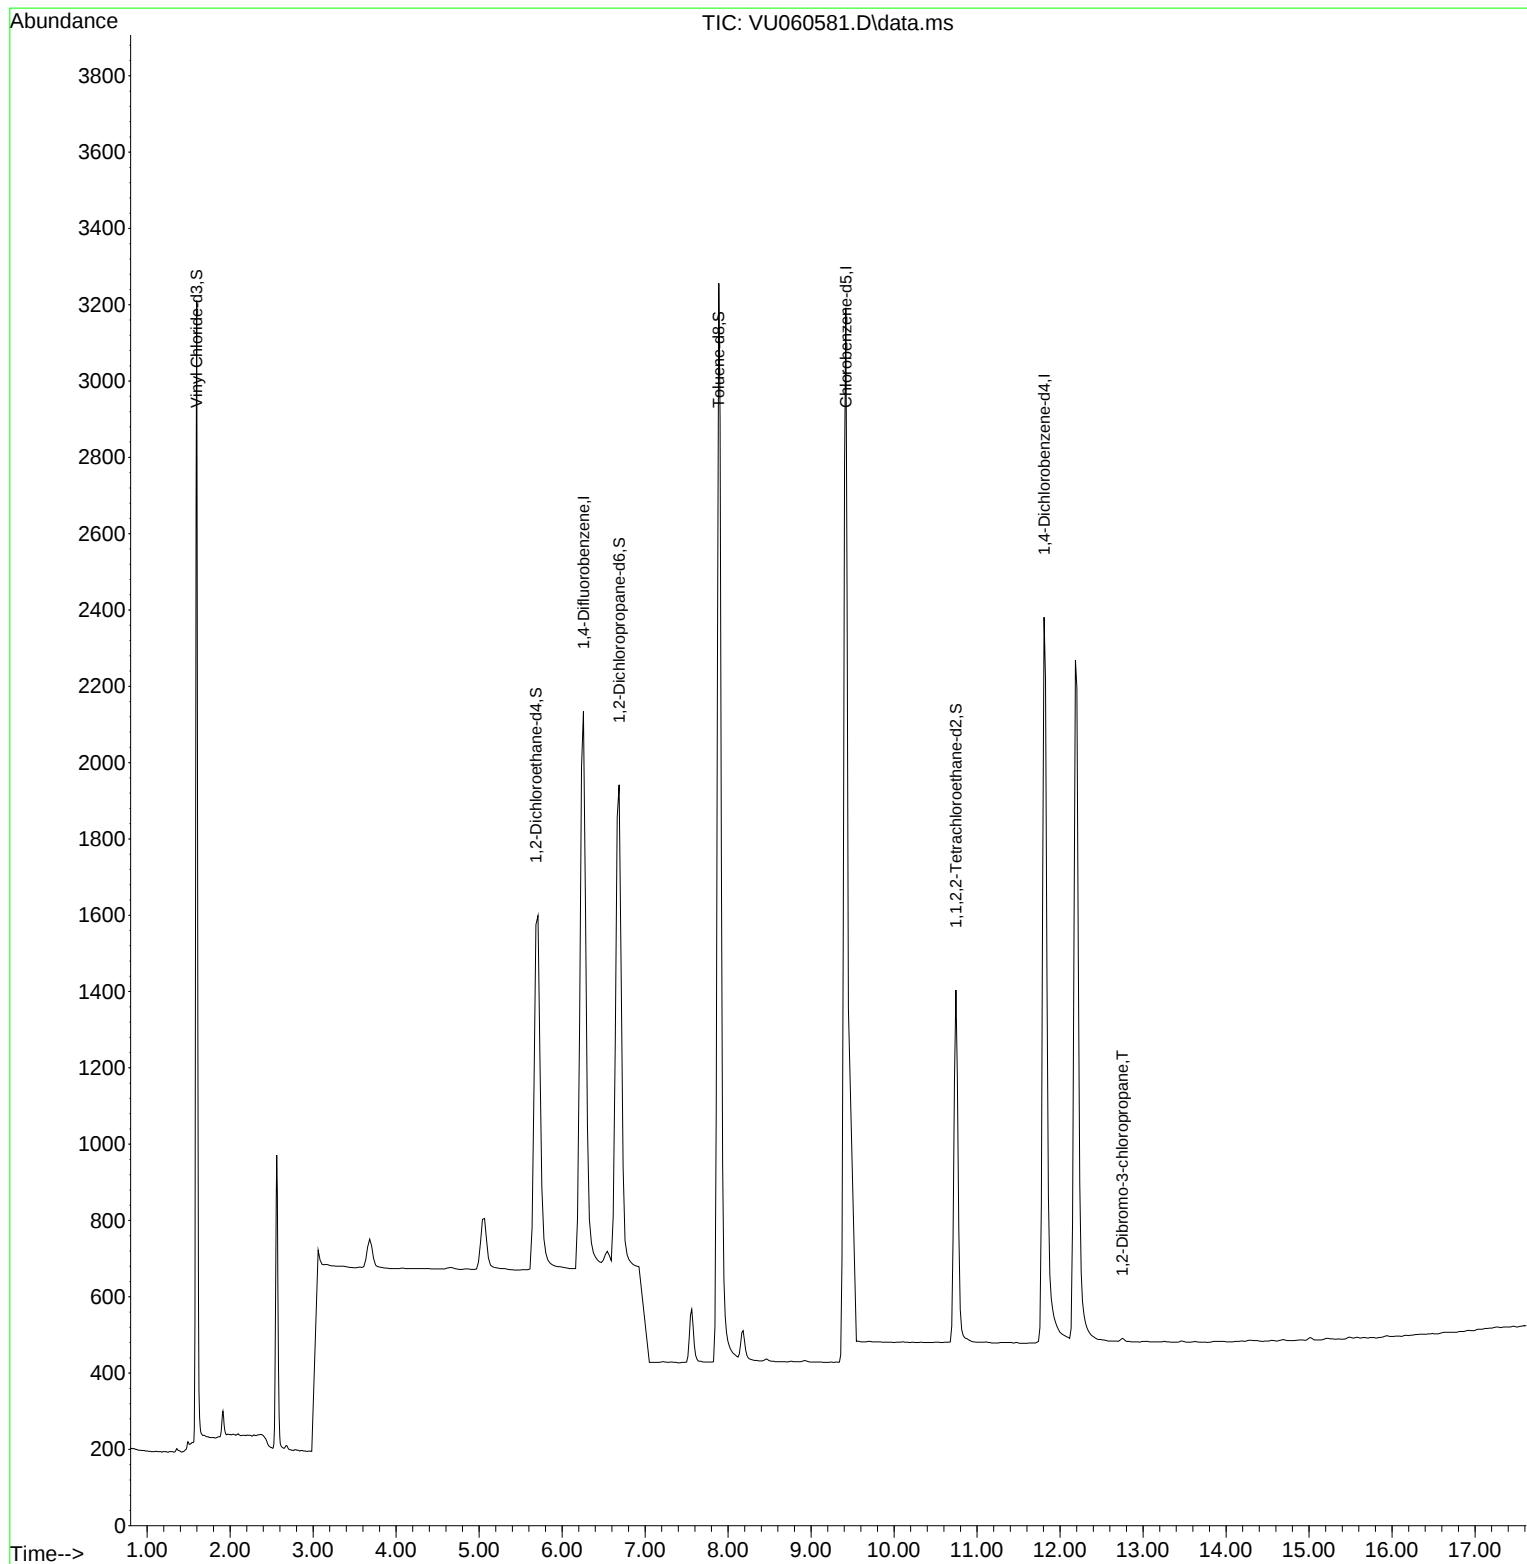

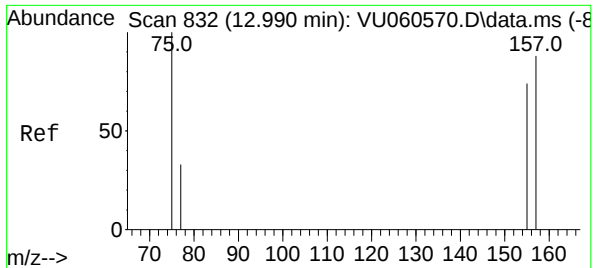

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.039 ug/L
 RT: 12.750 min Scan# 81
 Delta R.T. -0.240 min
 Lab File: VU060581.D
 Acq: 30 Aug 2024 18:09

Instrument :
 MSVOA_U
 ClientSampleId :

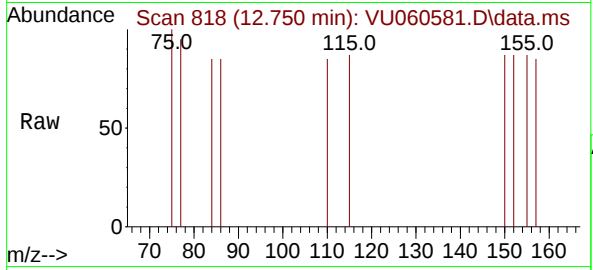

Tgt Ion: 75	Resp: 20
Ion Ratio	Lower Upper
75 100	
157 85.5	74.3 111.5
155 87.3	66.2 99.2

