

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060582.D
 Acq On : 30 Aug 2024 18:33
 Operator : MD/SY
 Sample : VSTDCCC0.5EC
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 01:03:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5260	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7867	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2287	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3337	0.390	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	78.000%		
4) 1,2-Dichloroethane-d4	5.685	65	2123	0.468	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2298	0.470	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	94.000%		
8) Toluene-d8	7.888	98	5328	0.527	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	106.000%		
10) 1,1,2,2-Tetrachloroeth...	10.746	84	1853	0.433	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	86.000%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.597	62	3627	0.404	ug/L	99
6) Trichloroethene	6.544	95	2173	0.437	ug/L	98
9) 1,2-Dibromoethane	8.924	107	1506	0.483	ug/L	100
12) 1,2,3-Trichloropropane	10.814	75	1335	0.503	ug/L	98
13) 1,2-Dibromo-3-chloropr...	12.991	75	257	0.499	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060582.D
Acq On : 30 Aug 2024 18:33
Operator : MD/SY
Sample : VSTDCCC0.5EC
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 31 01:03:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration




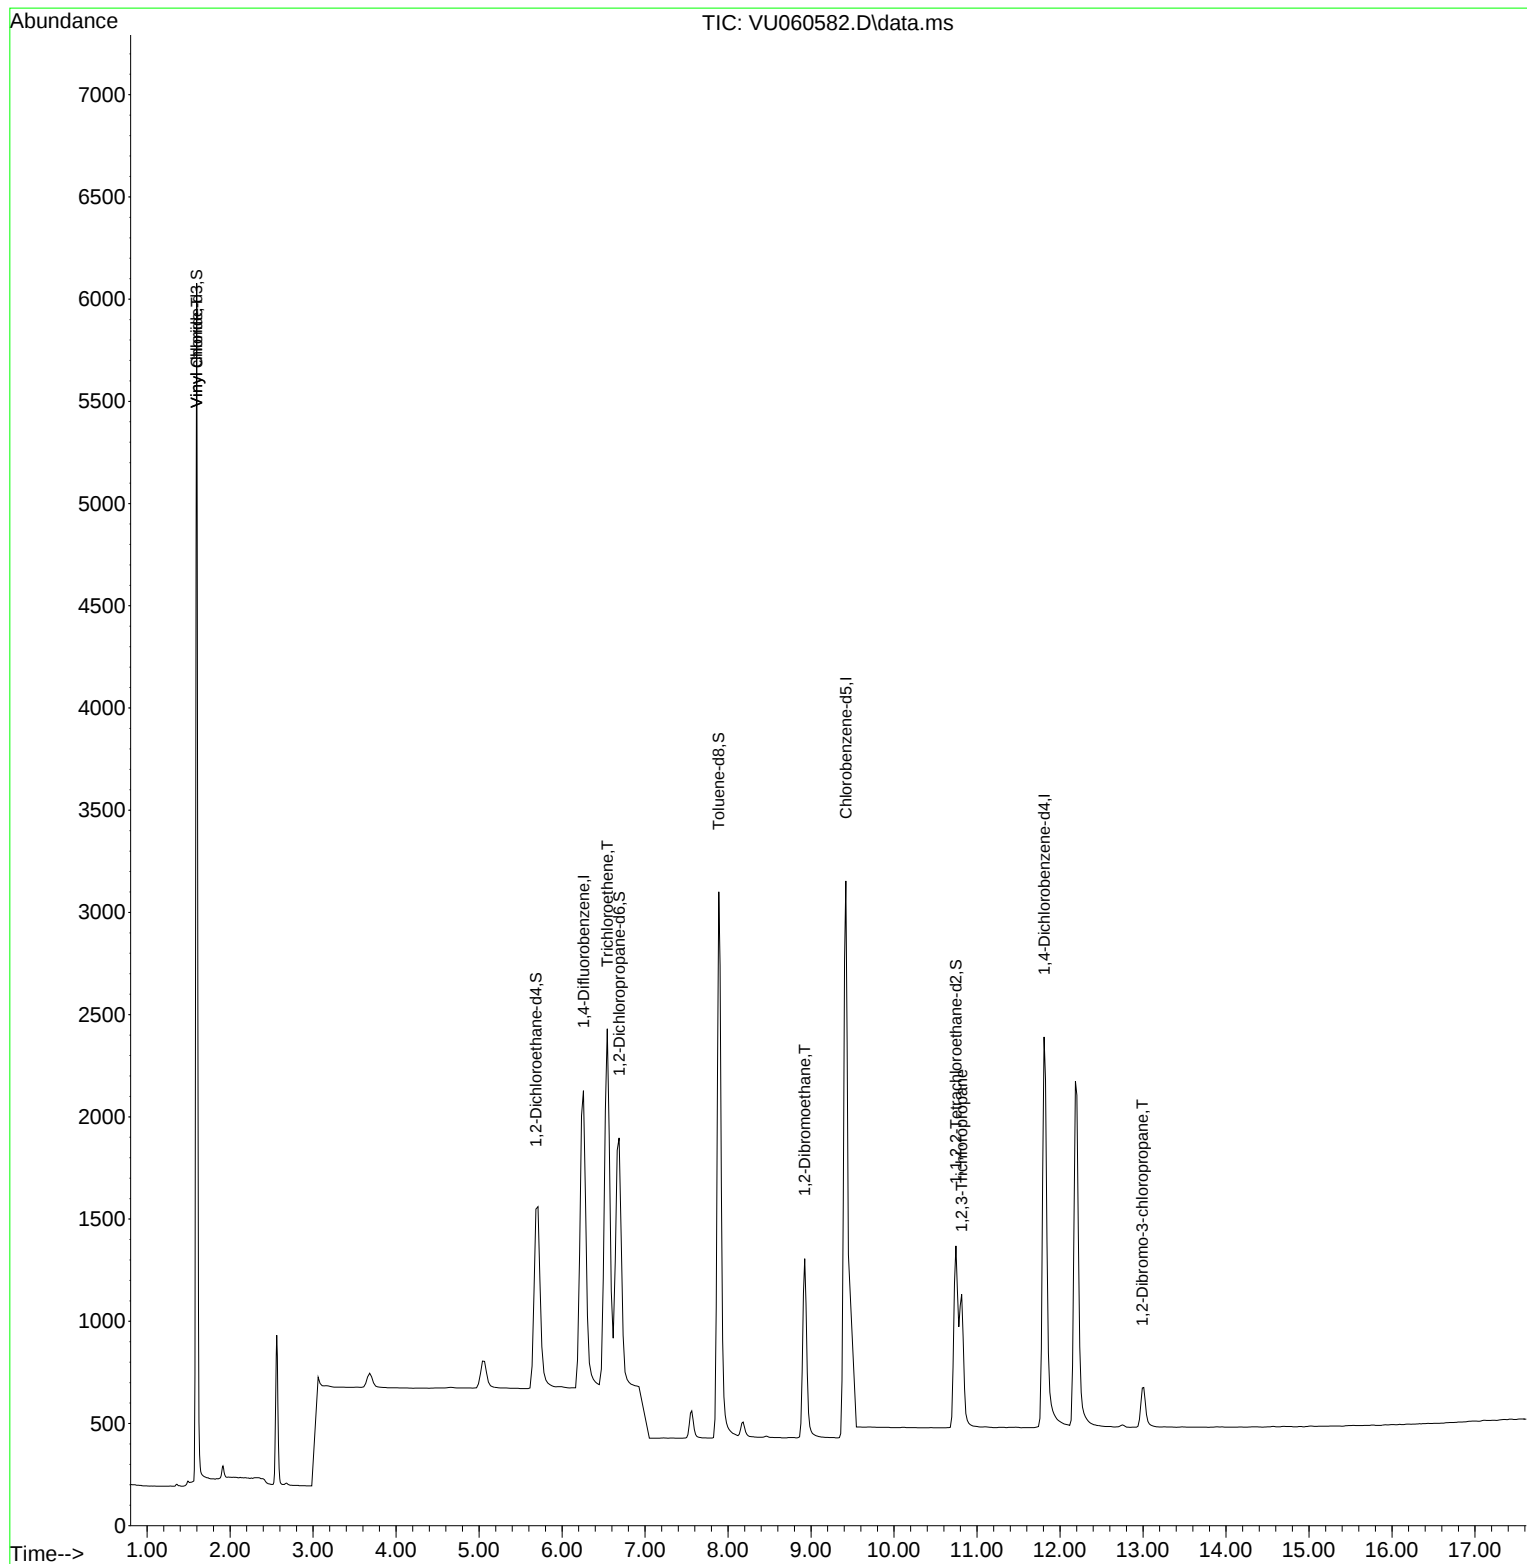


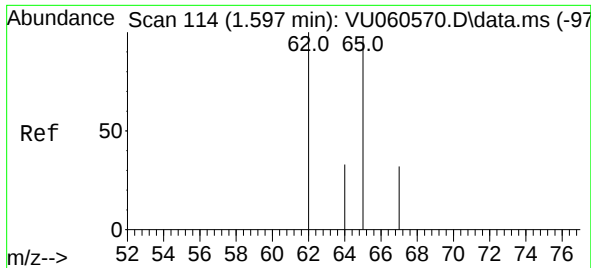

#3
 Vinyl chloride
 Concen: 0.404 ug/L
 RT: 1.597 min Scan# 114
 Delta R.T. 0.000 min
 Lab File: VU060582.D
 Acq: 30 Aug 2024 18:33




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 62 Resp: 3627
 Ion Ratio Lower Upper
 62 100
 64 34.7 23.9 44.3

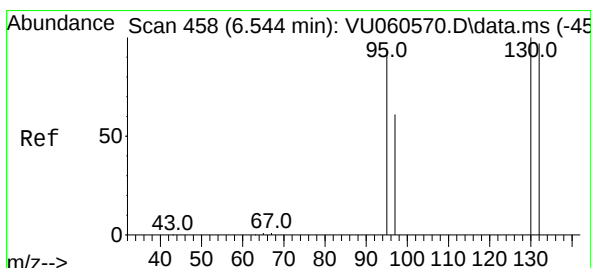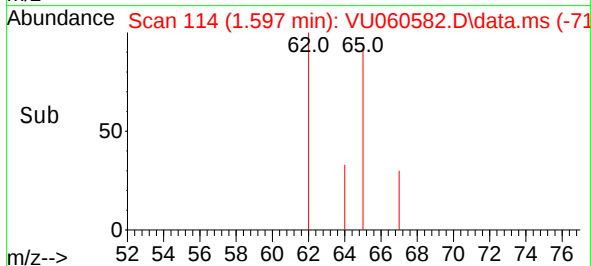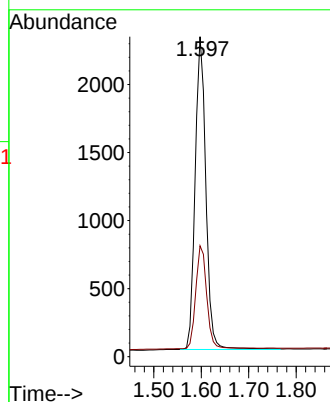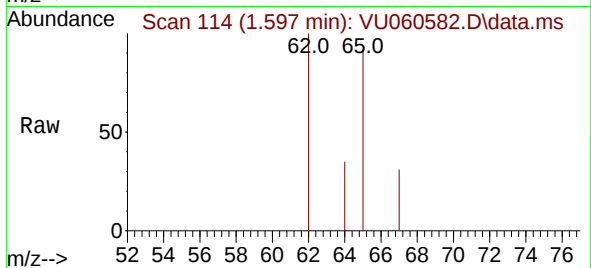

#6
 Trichloroethene
 Concen: 0.437 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU060582.D
 Acq: 30 Aug 2024 18:33


Tgt Ion: 95 Resp: 2173
 Ion Ratio Lower Upper
 95 100
 97 69.2 48.5 90.1
 132 104.7 75.5 140.1
 130 106.9 76.3 141.7

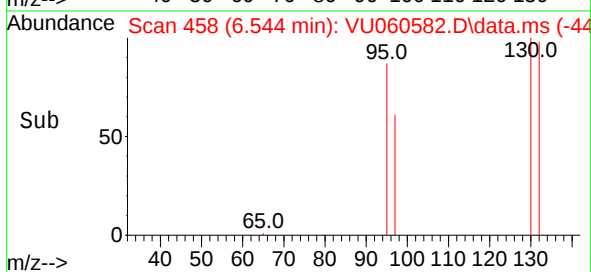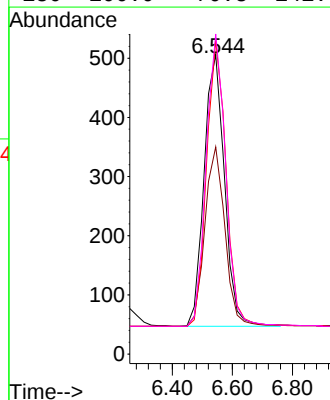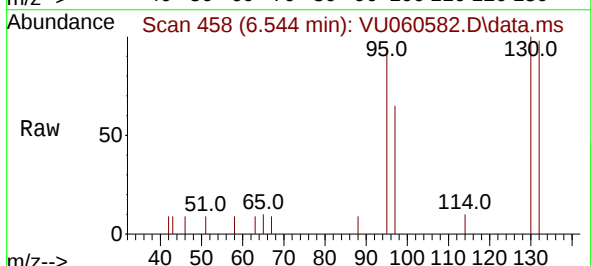



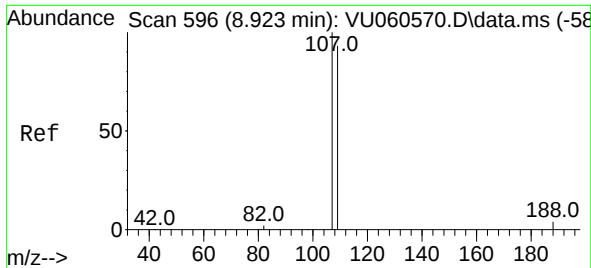


#9
1,2-Dibromoethane
Concen: 0.483 ug/L
RT: 8.924 min Scan# 596
Delta R.T. 0.000 min
Lab File: VU060582.D
Acq: 30 Aug 2024 18:33

Instrument :
MSVOA_U
ClientSampleId :



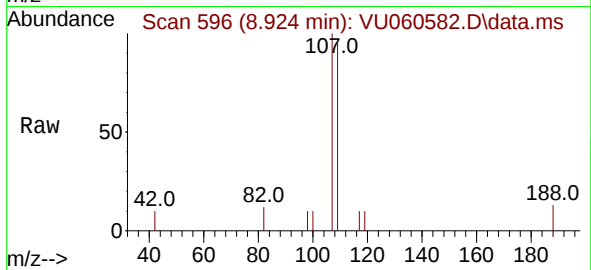



Tgt Ion:107 Resp: 1506
Ion Ratio Lower Upper
107 100
109 95.0 66.5 123.5
188 13.3 9.6 14.4

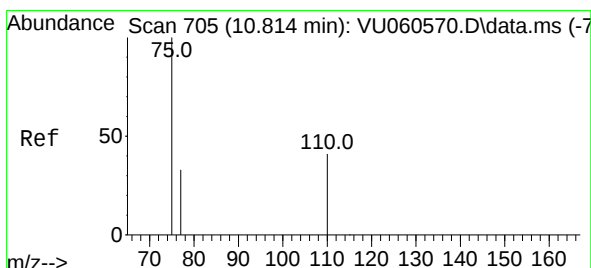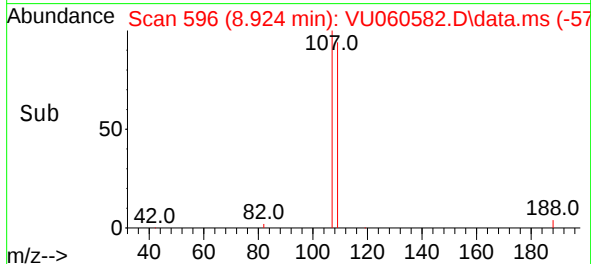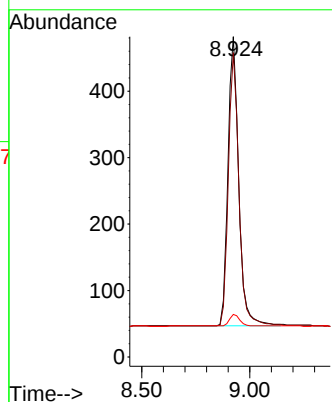

#12
1,2,3-Trichloropropane
Concen: 0.503 ug/L
RT: 10.814 min Scan# 705
Delta R.T. 0.000 min
Lab File: VU060582.D
Acq: 30 Aug 2024 18:33


Tgt Ion: 75 Resp: 1335
Ion Ratio Lower Upper
75 100
110 38.4 32.4 48.6
77 32.3 26.0 39.0

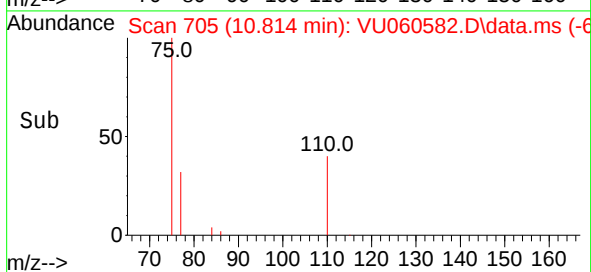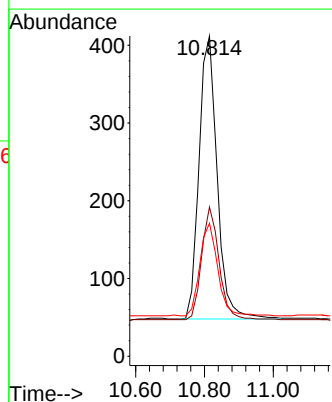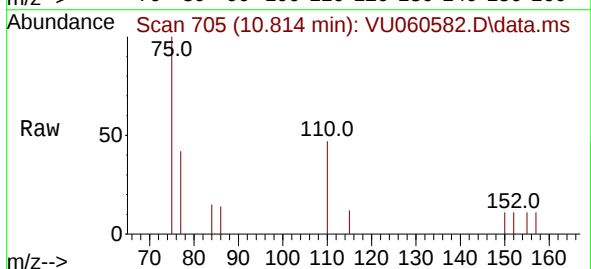

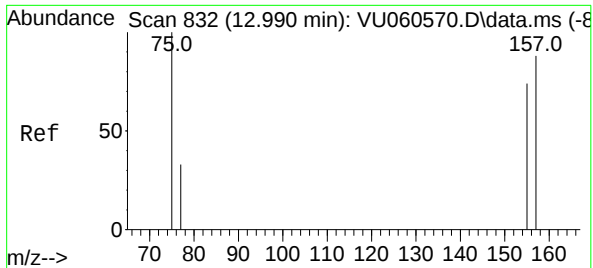

#13
1,2-Dibromo-3-chloropropane
Concen: 0.499 ug/L
RT: 12.991 min Scan# 84
Delta R.T. 0.000 min
Lab File: VU060582.D
Acq: 30 Aug 2024 18:33

Instrument :
MSVOA_U
ClientSampleId :

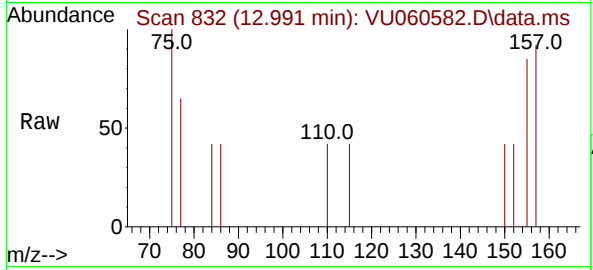

Tgt Ion: 75	Resp: 257
Ion Ratio	Lower Upper
75	100
157	92.0 74.3 111.5
155	85.0 66.2 99.2

