

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
 Data File : VU060576.D
 Acq On : 30 Aug 2024 16:32
 Operator : MD/SY
 Sample : P3803-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 OWBR-03-138-082924-VC

Quant Time: Aug 31 01:02:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	5467	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	8379	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2625	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	3739	0.420	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	84.000%
4) 1,2-Dichloroethane-d4	5.685	65	2288	0.486	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
7) 1,2-Dichloropropane-d6	6.687	67	2543	0.488	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	98.000%
8) Toluene-d8	7.887	98	5941	0.552	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2102	0.461	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	92.000%
Target Compounds						
3) Vinyl chloride	1.597	62	467	0.050	ug/L	Qvalue # 50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060576.D
Acq On : 30 Aug 2024 16:32
Operator : MD/SY
Sample : P3803-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
OWBR-03-138-082924-VC

Quant Time: Aug 31 01:02:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

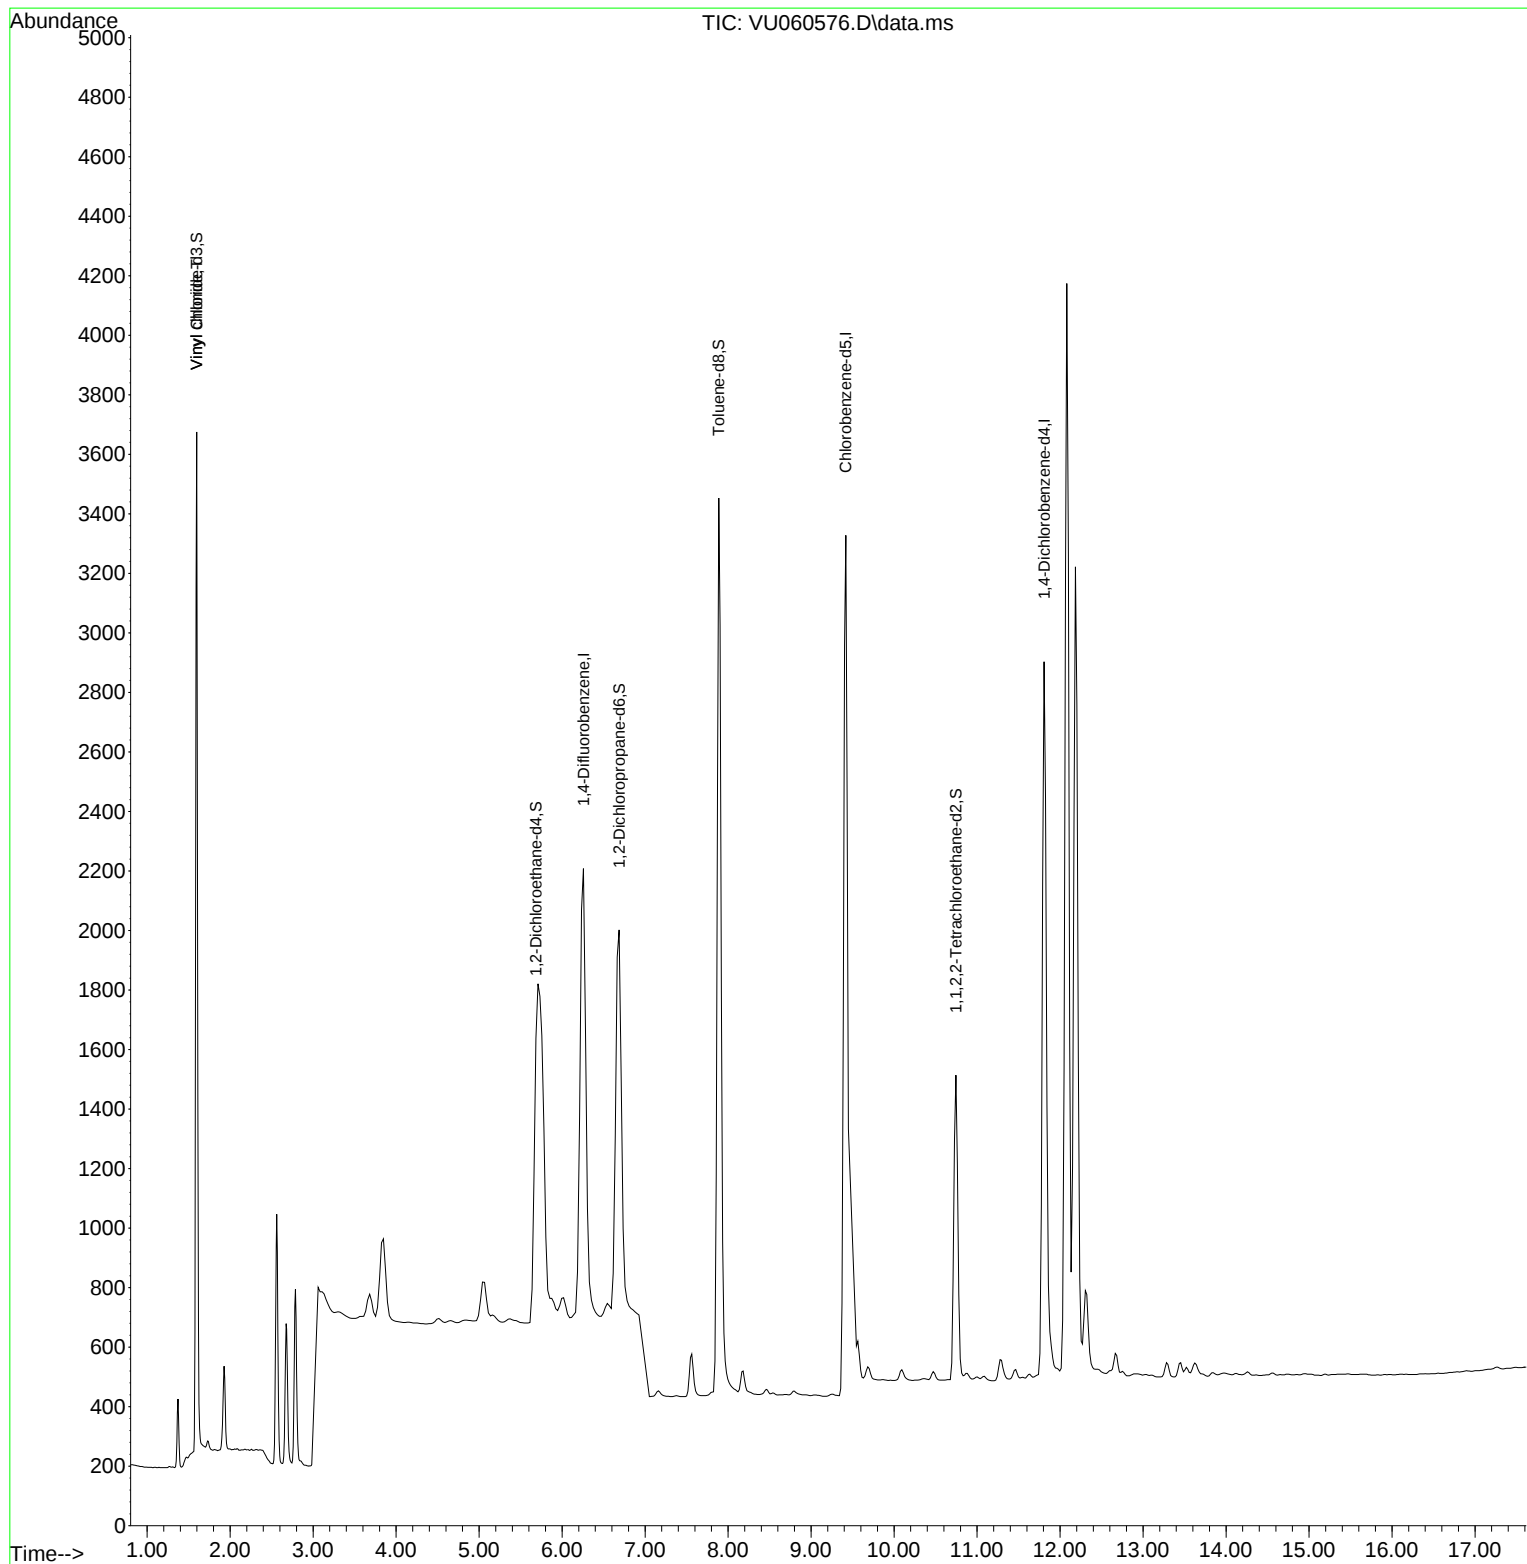

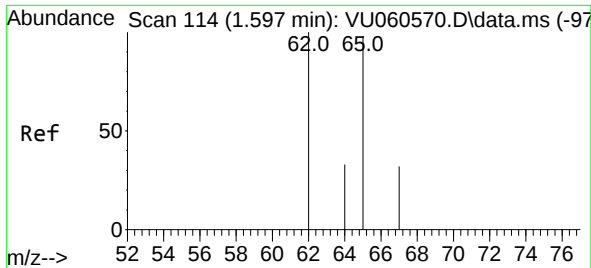

#3

Vinyl chloride

Concen: 0.050 ug/L

RT: 1.597 min Scan# 11

Delta R.T. 0.000 min

Lab File: VU060576.D


Acq: 30 Aug 2024 16:32

Instrument :

MSVOA_U

ClientSampleId :

OWBR-03-138-082924-VC

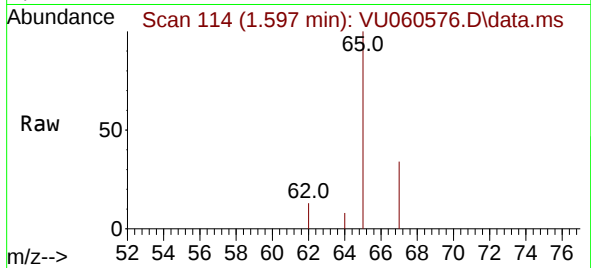

Tgt Ion: 62 Resp: 467

Ion Ratio Lower Upper

62 100

64 63.1 23.9 44.3#

