


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083024\
Data File : VU060569.D
Acq On : 30 Aug 2024 09:54
Operator : MD/SY
Sample : BFB013
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB013

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 05:03:57 2024

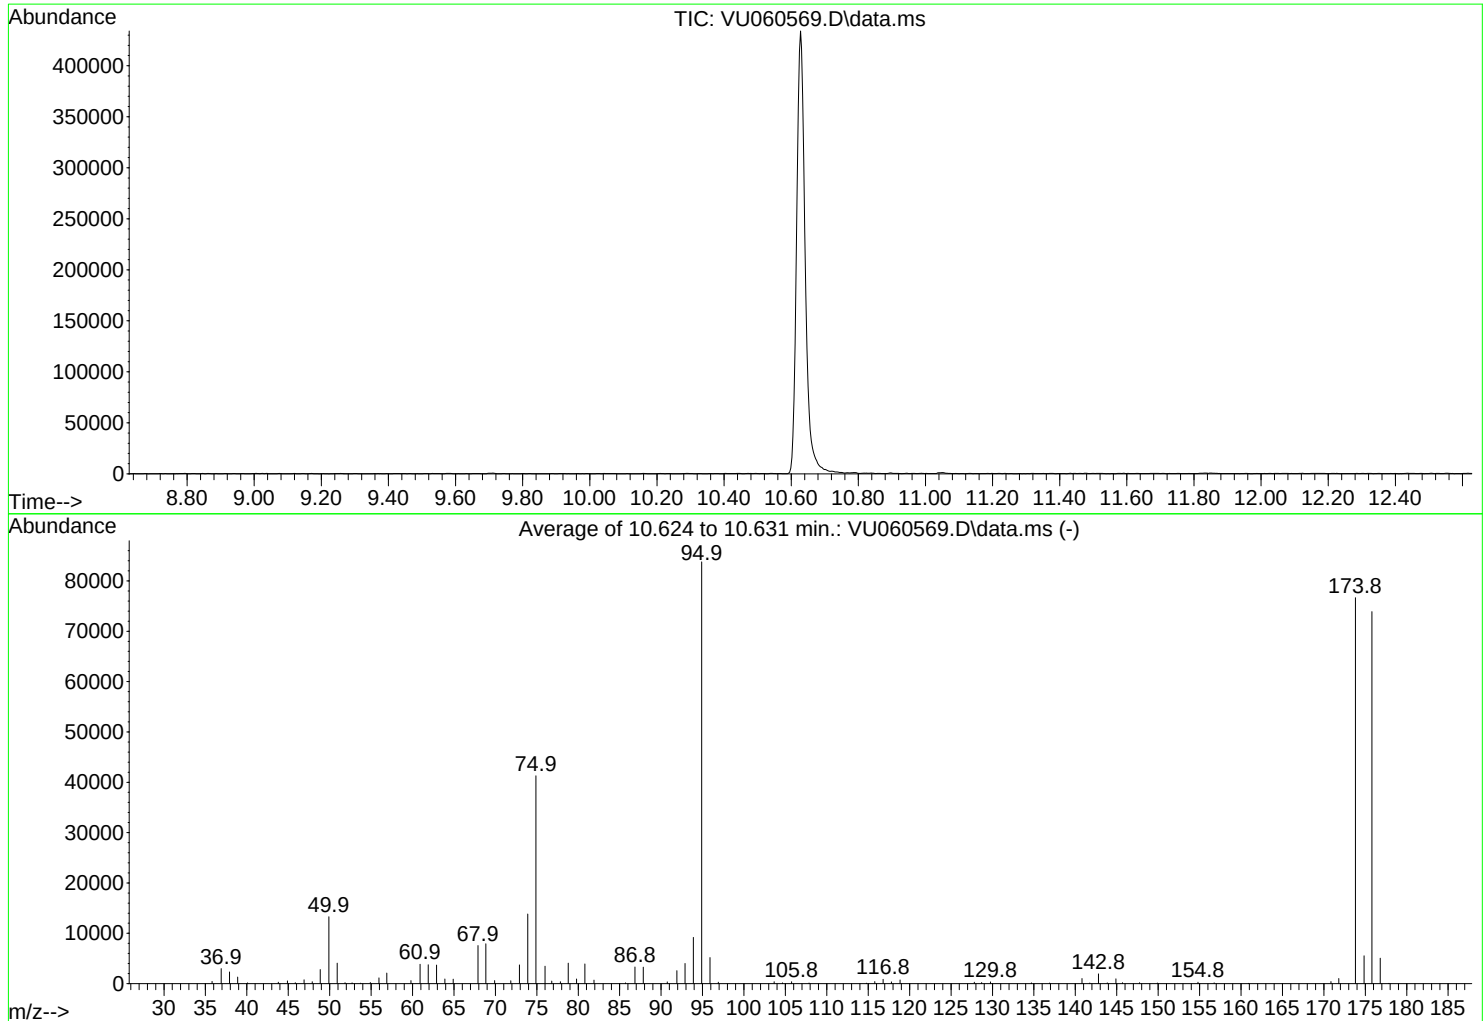

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13292	PASS
75	95	30	80	49.3	41291	PASS
95	95	100	100	100.0	83789	PASS
96	95	5	9	6.2	5175	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.5	76661	PASS
175	174	5	9	7.2	5537	PASS
176	174	95	101	96.4	73899	PASS
177	176	5	9	6.8	5058	PASS

m/z	Abundance
43.70	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	438.0
36.90	3094.0
37.90	2339.0
38.90	1317.0
40.10	134.0
43.90	543.0
44.90	563.0
45.80	171.0
46.90	753.0
48.00	354.0
48.90	2876.0
49.90	13611.0
50.90	4332.0
51.90	245.0
52.70	127.0
53.70	139.0
54.90	189.0
56.00	1095.0
56.90	2035.0
59.80	575.0
60.90	3844.0
61.90	3662.0
62.90	3595.0
63.90	920.0
64.90	855.0
67.90	7518.0
68.80	7785.0
69.90	686.0
71.90	613.0
72.90	3596.0
73.90	13891.0
74.90	40688.0
76.00	3550.0
76.80	498.0
77.90	360.0
78.80	4099.0
79.80	959.0
80.80	3820.0
81.90	644.0
85.70	157.0
86.90	3251.0
87.90	3284.0
90.70	356.0
91.90	2729.0
92.90	3874.0
93.90	8847.0
94.90	83200.0
95.90	5339.0
96.90	300.0
103.70	360.0
104.60	138.0
105.80	402.0
114.80	143.0
115.80	394.0
116.80	800.0
117.80	423.0
118.80	713.0
127.90	290.0
128.70	203.0
129.80	367.0
134.70	124.0
136.90	121.0
140.80	1003.0
141.80	140.0
142.80	1958.0
143.90	148.0
144.90	871.0
145.70	151.0
147.70	184.0
149.90	124.0
154.90	307.0
156.80	161.0
170.80	406.0
171.80	941.0
173.80	73720.0
174.90	5344.0
175.80	70632.0
176.80	4959.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	452.0
36.90	3078.0
37.90	2386.0
38.90	1348.0
40.10	181.0
43.90	510.0
44.90	556.0
45.90	196.0
46.90	794.0
47.90	392.0
48.90	2890.0
49.90	13609.0
50.90	4107.0
51.80	204.0
52.70	196.0
53.80	119.0
54.90	229.0
56.00	1185.0
56.90	2231.0
59.80	595.0
60.90	4015.0
61.90	3776.0
62.90	3817.0
63.90	945.0
64.90	921.0
67.90	7849.0
68.90	8175.0
69.90	641.0
71.90	618.0
72.90	3788.0
73.90	14055.0
74.90	42624.0
76.00	3522.0
76.80	492.0
77.80	415.0
78.80	4194.0
79.80	1011.0
80.80	4049.0
81.90	732.0
85.70	180.0
86.90	3416.0
87.80	3358.0
90.70	352.0
91.90	2649.0
92.90	4252.0
93.90	9508.0
94.90	86056.0
95.90	5381.0
96.90	295.0
103.70	387.0
104.70	163.0
105.80	410.0
107.90	149.0
114.80	137.0
115.80	423.0
116.80	899.0
117.80	342.0
118.90	745.0
127.80	291.0
128.70	222.0
129.80	367.0
134.70	174.0
136.90	141.0
140.80	1050.0
141.70	151.0
142.80	2011.0
143.90	161.0
144.90	1000.0
145.70	196.0
147.70	188.0
149.90	126.0
154.80	317.0
156.70	174.0
160.90	121.0
170.90	423.0
171.80	1013.0
173.80	78824.0
174.80	5639.0
175.80	76160.0
176.80	5232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.70	455.0
36.90	2816.0
37.90	2266.0
38.90	1228.0
40.10	176.0
43.90	494.0
44.90	499.0
45.90	163.0
46.90	746.0
47.80	442.0
48.80	2680.0
49.90	12657.0
50.90	3750.0
51.90	150.0
52.70	177.0
54.90	221.0
55.90	1126.0
56.90	2023.0
59.80	627.0
60.90	3727.0
61.90	3800.0
62.90	3637.0
63.90	886.0
64.90	942.0
67.90	7312.0
68.90	7800.0
69.90	529.0
71.80	512.0
72.90	3810.0
73.90	13498.0
74.90	40560.0
76.00	3318.0
76.80	523.0
77.80	347.0
78.80	3948.0
79.80	839.0
80.80	3831.0
81.90	710.0
85.70	145.0
86.80	3270.0
87.80	3192.0
90.80	319.0
91.90	2392.0
92.90	3908.0
93.90	9240.0
94.90	82112.0
95.90	4804.0
96.90	234.0
103.60	404.0
104.70	147.0
105.70	373.0
107.80	213.0
115.80	397.0
116.80	882.0
117.80	278.0
118.90	784.0
127.70	305.0
128.70	201.0
129.70	312.0
134.70	216.0
136.90	146.0
140.80	1016.0
141.70	136.0
142.80	1873.0
143.80	160.0
144.90	1039.0
145.70	209.0
147.80	211.0
149.90	107.0
154.70	272.0
156.70	187.0
160.90	127.0
170.90	414.0
171.80	1114.0
173.80	77440.0
174.80	5627.0
175.80	74904.0
176.80	4982.0
177.80	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013