


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083118\
 Data File : VU026485.D
 Acq On : 31 Aug 2018 08:56
 Operator : MD/SY
 Sample : BFB47
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 01 06:27:57 2018

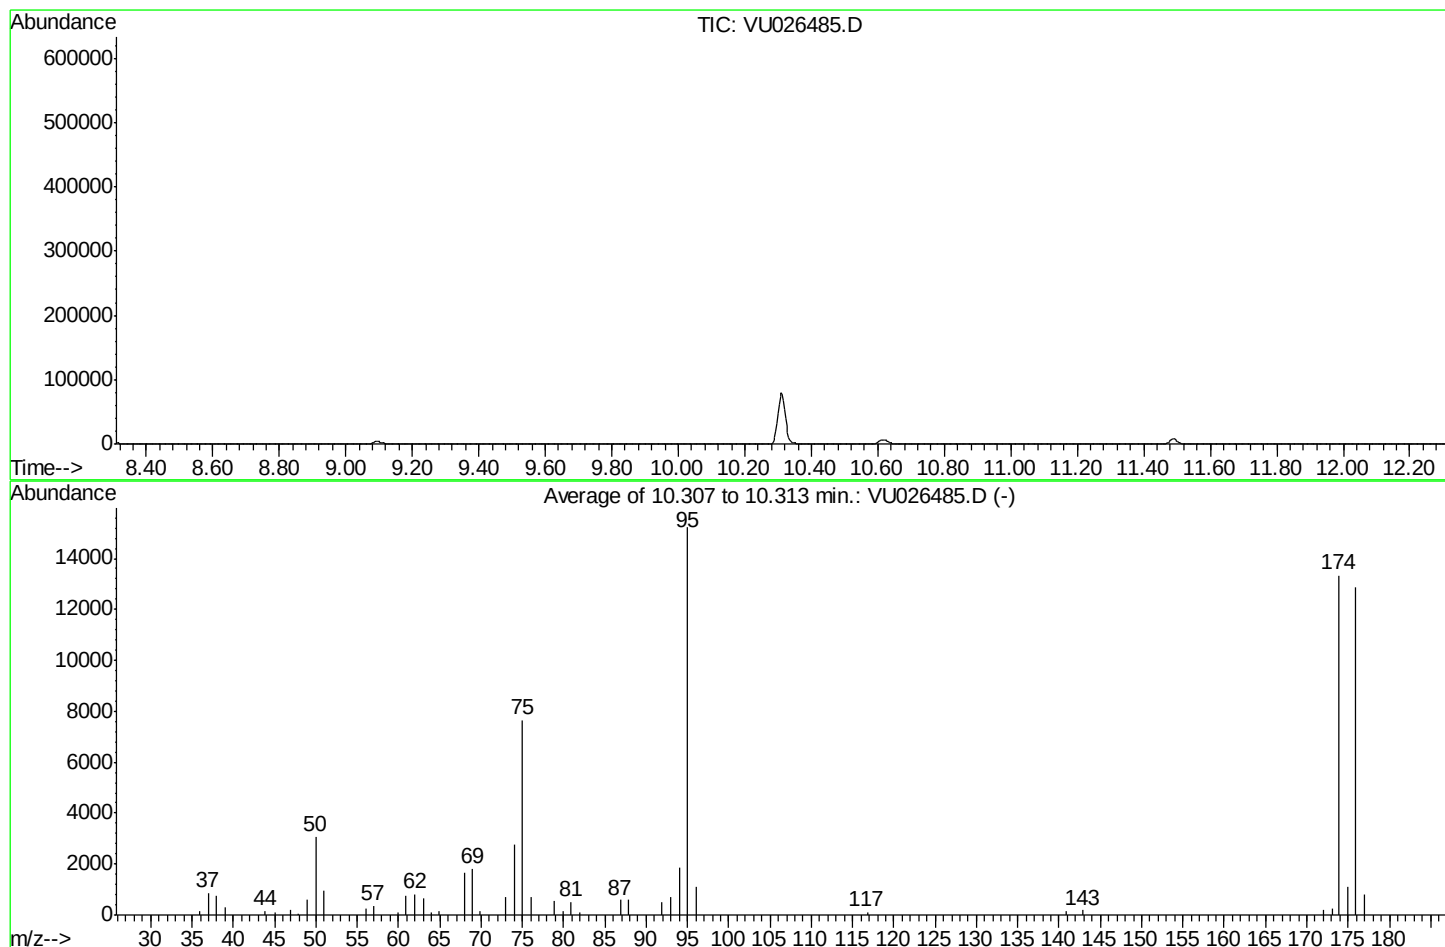

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	3087	PASS
75	95	30	80	50.3	7664	PASS
95	95	100	100	100.0	15224	PASS
96	95	5	9	7.3	1107	PASS
173	174	0.00	2	1.7	231	PASS
174	95	50	120	87.6	13330	PASS
175	174	5	9	8.5	1130	PASS
176	174	95	101	96.6	12875	PASS
177	176	5	9	6.4	828	PASS

Scan 3011 (10.271 min): VU026485.D
BFB47

m/z	Abundance
44.00	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.00	128.0
37.00	814.0
38.00	724.0
39.00	305.0
43.00	388.0
45.00	136.0
47.00	148.0
47.00	106.0
49.00	597.0
50.00	3000.0
51.00	869.0
56.00	258.0
57.00	385.0
60.00	118.0
60.00	670.0
62.00	802.0
63.00	679.0
63.00	133.0
65.00	154.0
68.00	1630.0
69.00	1694.0
69.00	141.0
72.00	692.0
74.00	2688.0
75.00	7260.0
76.00	695.0
78.00	539.0
79.00	125.0
80.00	541.0
81.00	113.0
86.00	580.0
87.00	526.0
91.00	449.0
93.00	679.0
94.00	1859.0
95.00	14777.0
96.00	1069.0
116.00	109.0
140.00	146.0
142.00	170.0
171.00	195.0
173.00	214.0
173.00	12632.0
174.00	1150.0
175.00	12154.0
176.00	771.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.00	150.0
37.00	926.0
38.00	792.0
39.00	285.0
43.00	379.0
45.00	111.0
46.00	192.0
49.00	625.0
50.00	3199.0
51.00	988.0
56.00	251.0
57.00	365.0
60.00	115.0
61.00	768.0
62.00	845.0
63.00	632.0
63.00	129.0
65.00	138.0
68.00	1708.0
69.00	1929.0
69.00	154.0
72.00	778.0
74.00	2819.0
75.00	7901.0
76.00	723.0
78.00	565.0
79.00	146.0
80.00	532.0
81.00	120.0
86.00	602.0
87.00	600.0
91.00	497.0
93.00	727.0
94.00	1940.0
95.00	15737.0
96.00	1142.0
116.00	102.0
140.00	152.0
142.00	213.0
172.00	233.0
173.00	237.0
173.00	13786.0
174.00	1166.0
175.00	13285.0
176.00	863.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.90	167.0
37.00	893.0
38.00	763.0
39.00	298.0
43.90	340.0
46.90	204.0
49.00	605.0
50.00	3063.0
51.00	949.0
56.00	220.0
57.00	359.0
60.00	109.0
61.00	770.0
62.00	785.0
63.00	601.0
64.90	131.0
68.00	1645.0
69.00	1848.0
69.90	132.0
72.90	715.0
74.00	2735.0
75.00	7833.0
76.00	672.0
78.90	534.0
79.90	151.0
80.90	504.0
81.90	106.0
86.90	629.0
87.90	675.0
91.90	512.0
93.00	726.0
94.00	1779.0
95.00	15160.0
96.00	1111.0
116.80	103.0
140.80	162.0
142.90	199.0
172.00	229.0
173.10	243.0
173.90	13573.0
174.90	1076.0
175.90	13186.0
176.90	850.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47