


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU083120\
 Data File : VU039996.D
 Acq On : 31 Aug 2020 09:04
 Operator : SY/MD
 Sample : BFB24
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 31 18:16:59 2020

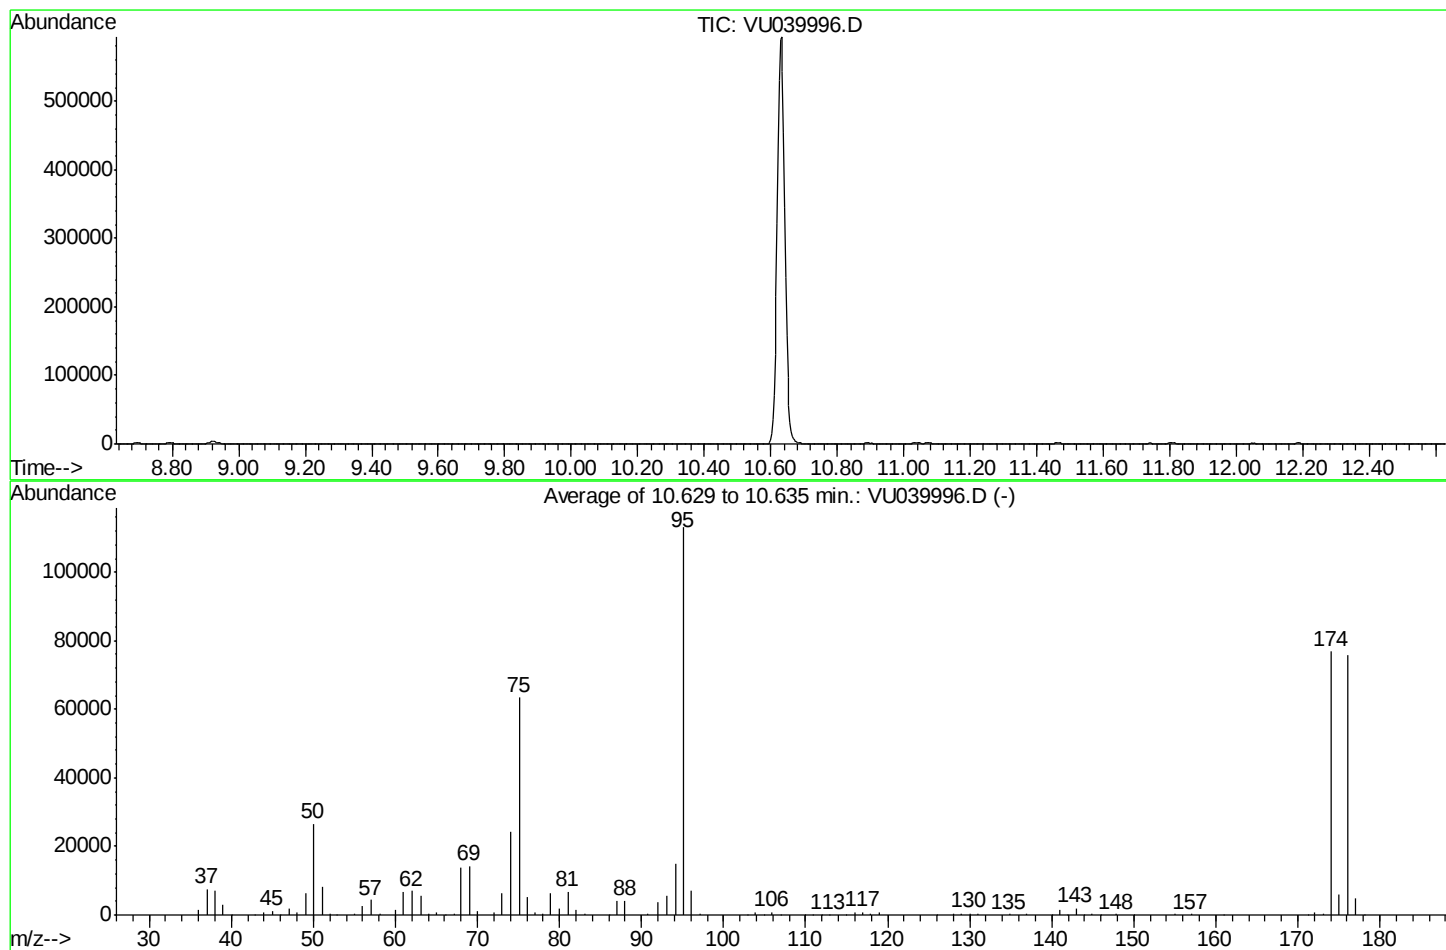

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	26701	PASS
75	95	30	80	56.0	63378	PASS
95	95	100	100	100.0	113088	PASS
96	95	5	9	6.4	7222	PASS
173	174	0.00	2	0.5	357	PASS
174	95	50	120	67.9	76802	PASS
175	174	5	9	7.9	6048	PASS
176	174	95	101	98.8	75850	PASS
177	176	5	9	6.5	4949	PASS

m/z	Abundance
36.00	1635.0
37.00	7738.0
38.00	7868.0
39.00	3152.0
40.10	227.0
42.90	141.0
44.00	1208.0
45.00	1265.0
45.90	222.0
47.00	1750.0
47.90	904.0
49.00	6718.0
50.00	27880.0
51.10	8563.0
52.00	316.0
52.80	124.0
55.10	506.0
56.00	2491.0
57.00	4576.0
58.10	257.0
60.00	1422.0
61.00	6973.0
62.00	7221.0
63.00	5721.0
64.00	606.0
65.00	761.0
66.10	169.0
67.20	438.0
68.00	14590.0
69.00	14951.0
70.00	1202.0
72.00	769.0
73.00	6440.0
74.00	25016.0
75.10	65792.0
76.00	5562.0
77.00	873.0
77.90	538.0
78.90	6493.0
79.90	2012.0
81.00	6817.0
82.00	1654.0
83.00	226.0
87.00	4410.0
88.00	4495.0
90.80	517.0
92.00	4008.0
93.00	5563.0
94.10	15397.0
95.10	115136.0
96.10	7692.0
97.10	191.0
102.90	117.0
103.90	762.0
104.90	203.0
105.90	882.0
110.00	154.0
110.80	112.0
112.00	161.0
112.80	168.0
114.80	240.0
116.00	618.0
117.00	963.0
118.00	477.0
119.00	857.0
126.00	103.0
128.10	348.0
128.90	243.0
130.00	432.0
131.00	217.0
134.90	363.0
137.00	206.0
141.00	1767.0
141.80	140.0
143.00	1996.0
144.80	242.0
146.00	197.0
147.90	312.0
150.10	141.0
155.00	242.0
157.00	248.0
161.00	128.0
172.00	949.0
173.10	1071.0
174.10	77512.0
175.00	6393.0
176.10	74704.0
177.00	4879.0
178.10	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1584.0
37.00	7845.0
38.00	7535.0
39.00	3176.0
40.10	171.0
42.90	124.0
44.00	1207.0
45.00	1235.0
45.90	180.0
47.00	1778.0
48.00	879.0
49.00	6674.0
50.00	27600.0
51.00	8673.0
52.00	344.0
55.00	479.0
56.00	2563.0
57.00	4643.0
58.10	233.0
60.00	1457.0
61.00	6644.0
62.00	7085.0
63.10	5532.0
64.00	571.0
65.00	761.0
66.00	134.0
67.10	483.0
68.00	14296.0
69.00	14808.0
70.00	1152.0
72.00	714.0
73.00	6628.0
74.00	25544.0
75.10	65104.0
76.00	5399.0
77.10	890.0
77.90	505.0
78.90	6431.0
79.90	2068.0
81.00	7096.0
82.00	1594.0
83.00	234.0
87.00	4191.0
88.00	4275.0
90.80	546.0
92.00	3825.0
93.00	5676.0
94.10	15529.0
95.10	116848.0
96.10	7300.0
97.10	252.0
102.90	124.0
103.90	730.0
104.90	200.0
105.90	889.0
110.00	120.0
110.80	103.0
112.00	164.0
112.90	176.0
114.90	203.0
116.00	610.0
117.00	974.0
117.90	561.0
119.00	734.0
128.10	359.0
128.90	272.0
130.00	440.0
131.00	216.0
134.90	362.0
136.90	233.0
141.00	1719.0
141.90	172.0
143.00	1967.0
144.00	173.0
144.90	217.0
145.90	169.0
147.90	395.0
150.10	179.0
155.00	253.0
157.00	287.0
161.00	153.0
171.30	222.0
172.10	896.0
174.10	79016.0
175.00	6292.0
176.10	78408.0
177.10	5142.0
178.10	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1302.0
37.00	7409.0
38.00	6401.0
39.00	2702.0
40.10	146.0
44.00	1170.0
45.00	1160.0
45.90	121.0
47.00	1583.0
48.00	850.0
49.10	6007.0
50.00	24624.0
51.00	7627.0
52.00	324.0
55.00	395.0
56.00	2433.0
57.00	4222.0
58.10	209.0
60.00	1319.0
61.00	6072.0
62.00	6467.0
63.00	5050.0
64.00	534.0
65.00	646.0
67.10	451.0
68.00	12663.0
69.00	13111.0
70.00	988.0
71.90	657.0
73.00	6051.0
74.00	22840.0
75.10	59240.0
76.10	4820.0
77.10	831.0
77.90	381.0
78.90	5802.0
79.90	1834.0
81.00	6731.0
81.90	1343.0
83.10	192.0
86.00	153.0
87.00	3806.0
87.90	3688.0
90.80	529.0
92.00	3471.0
93.10	5201.0
94.10	14314.0
95.10	107280.0
96.10	6676.0
97.10	252.0
103.90	670.0
104.90	182.0
105.90	784.0
106.90	127.0
111.90	174.0
112.90	250.0
114.90	154.0
116.00	604.0
117.00	877.0
117.80	556.0
119.00	609.0
128.10	329.0
128.90	275.0
130.00	364.0
130.90	197.0
134.80	266.0
136.90	237.0
140.00	110.0
141.00	1489.0
142.00	184.0
143.00	1682.0
144.00	215.0
144.90	164.0
145.90	142.0
147.90	365.0
150.10	158.0
155.00	205.0
157.10	270.0
161.00	118.0
171.20	201.0
172.10	766.0
174.10	73880.0
175.10	5461.0
176.10	74440.0
177.10	4827.0
178.10	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Scan 2875 (10.584 min): VU039996.D
BFB24

m/z	Abundance
40.00	113.0
43.90	294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24