

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050560.D
 Acq On : 31 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4363-06ME
 Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:19:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

09/01/2022
 Supervised By :Mahesh
 Dadoda

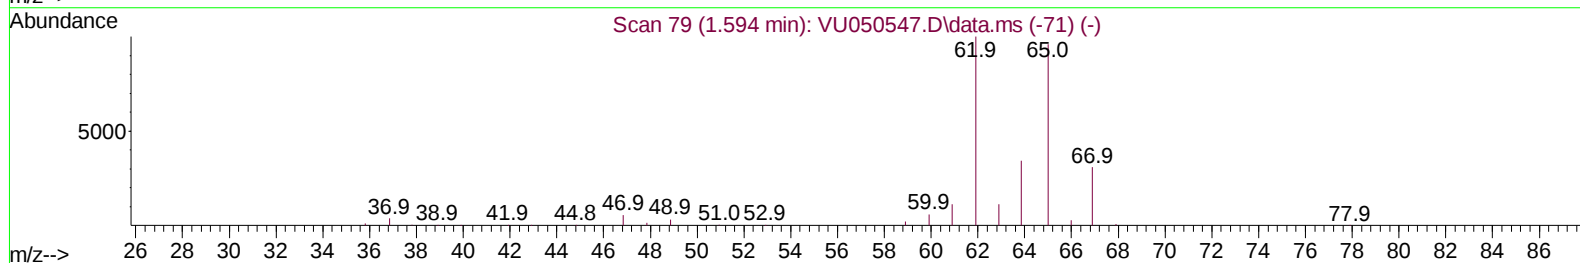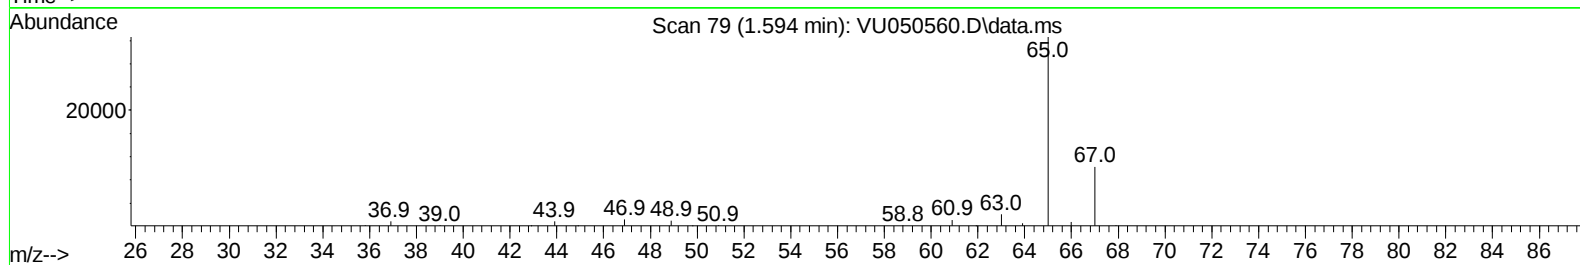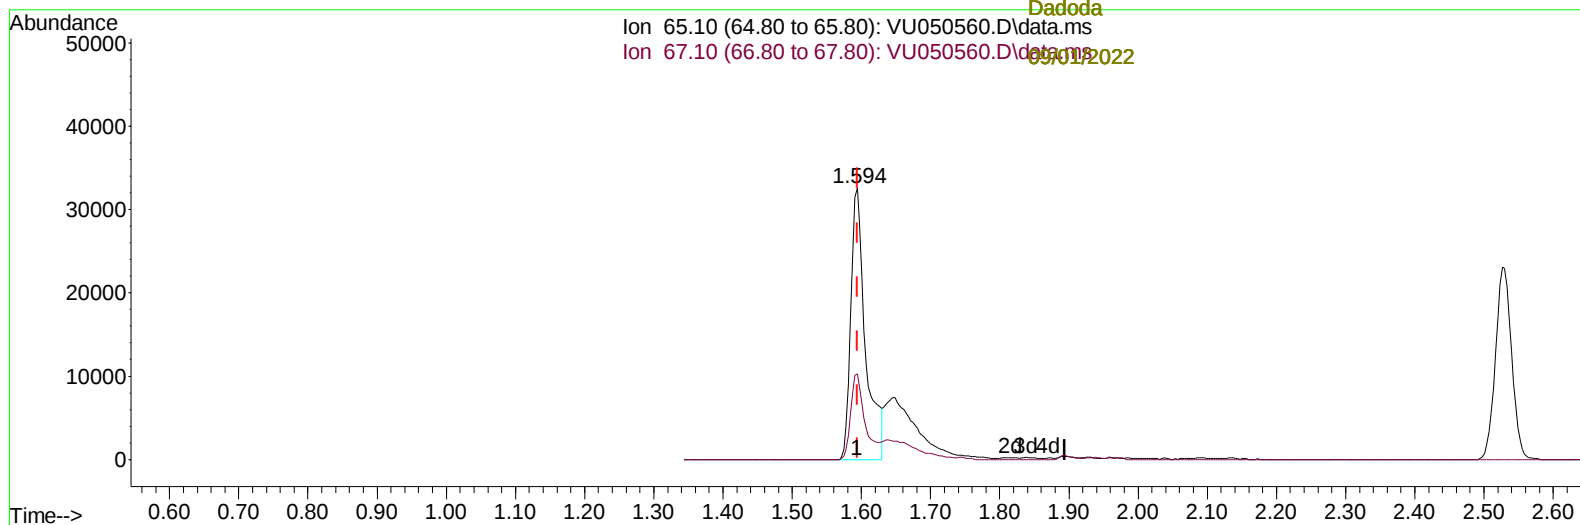

TIC: VU050560.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 24.27 ug/L

response 47736

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	30.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050560.D
 Acq On : 31 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4363-06ME
 Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW1ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa
 Patel

09/01/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Sep 01 05:19:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

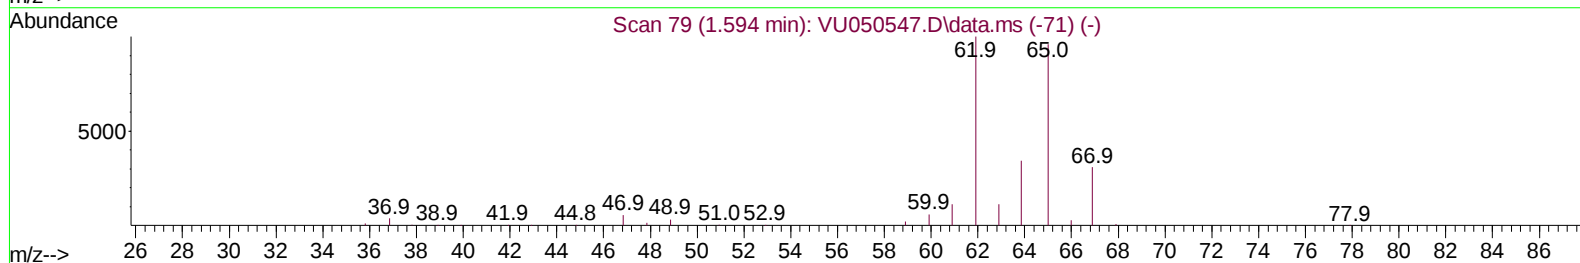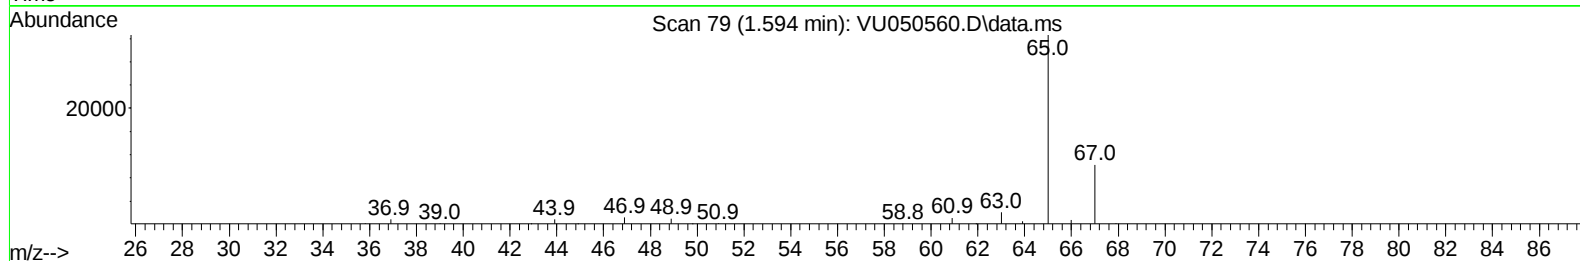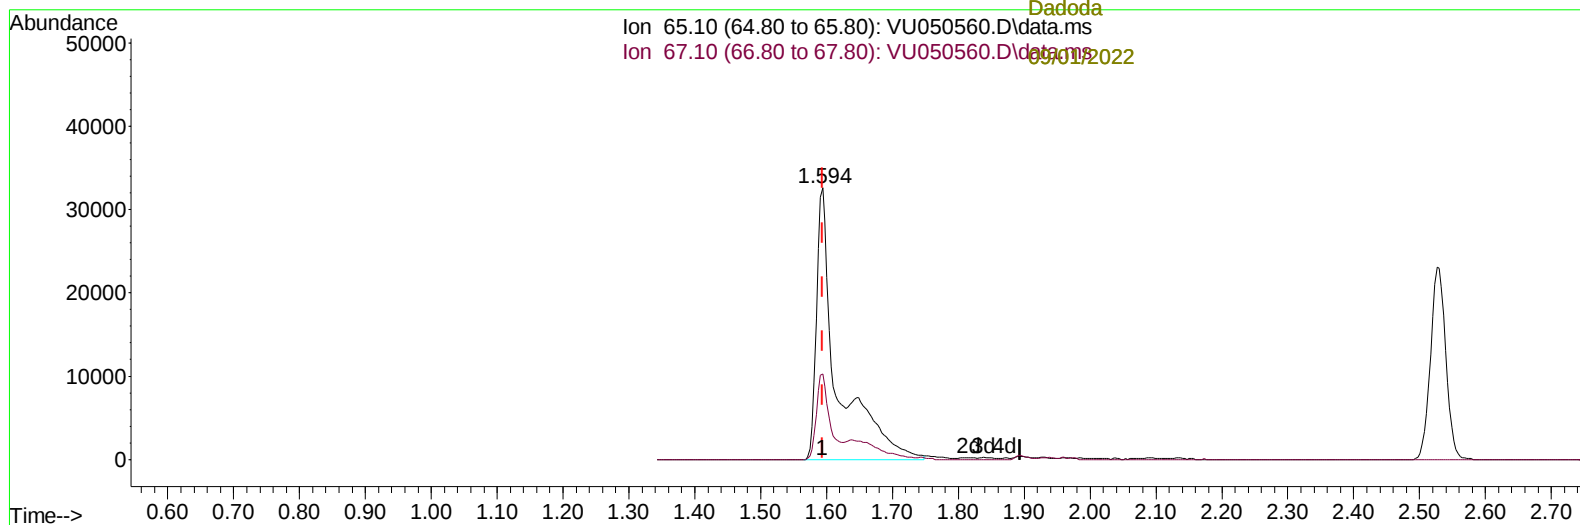

TIC: VU050560.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 36.46 ug/L m

response 71719

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	20.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050560.D
 Acq On : 31 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4363-06ME
 Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:19:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration




Reviewed By :Krupa
 Patel

09/01/2022
 Supervised By :Mahesh
 Dadoda

Ion 69.10 (68.80 to 69.80): VU050560.D\data.ms

Ion 71.10 (70.80 to 71.80): VU050560.D\data.ms

Ion 51.00 (50.70 to 51.70): VU050560.D\data.ms

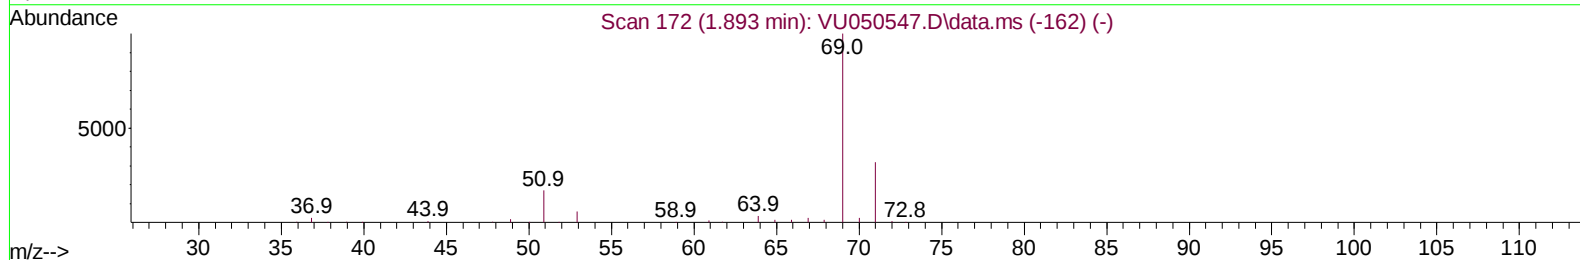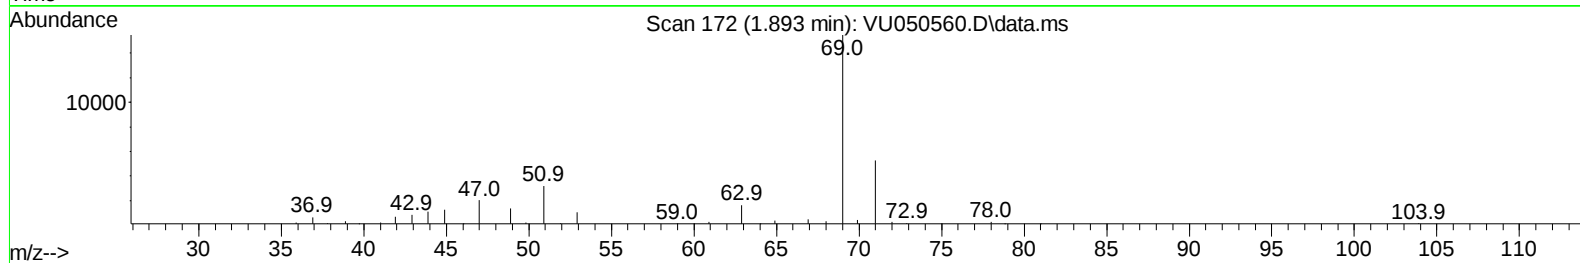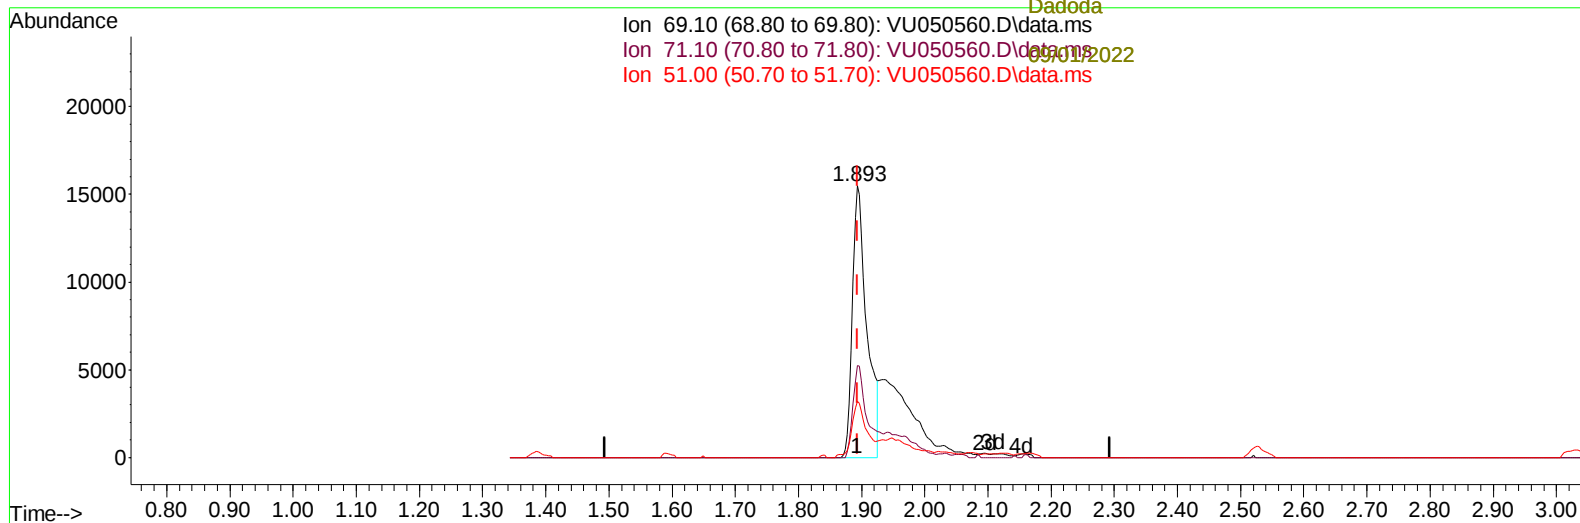

TIC: VU050560.D\data.ms

(7) Chloroethane-d5 (S)

1.893min (-0.000) 16.12 ug/L

response 24719

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	35.64
51.00	18.40	20.92
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050560.D
 Acq On : 31 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4363-06ME
 Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:19:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

09/01/2022
 Supervised By :Mahesh
 Dadoda

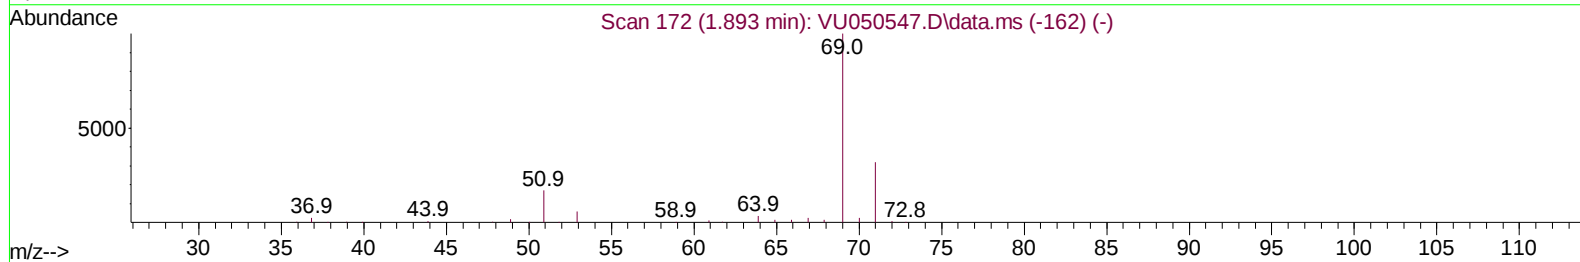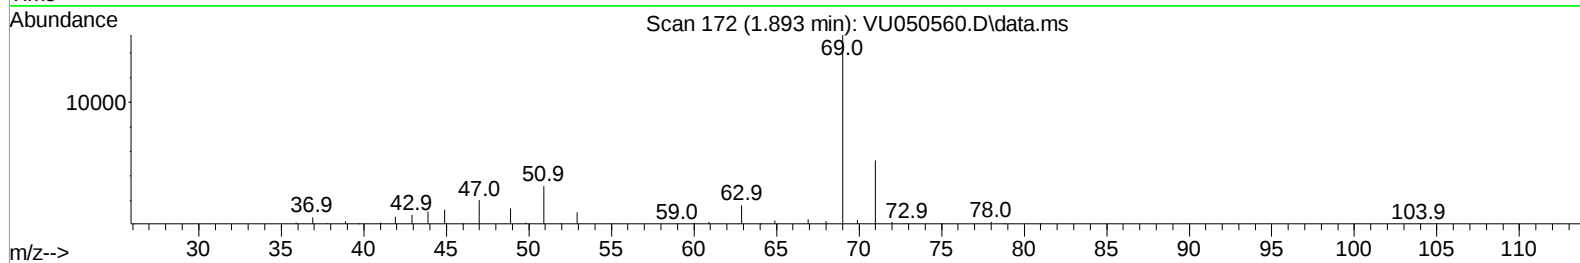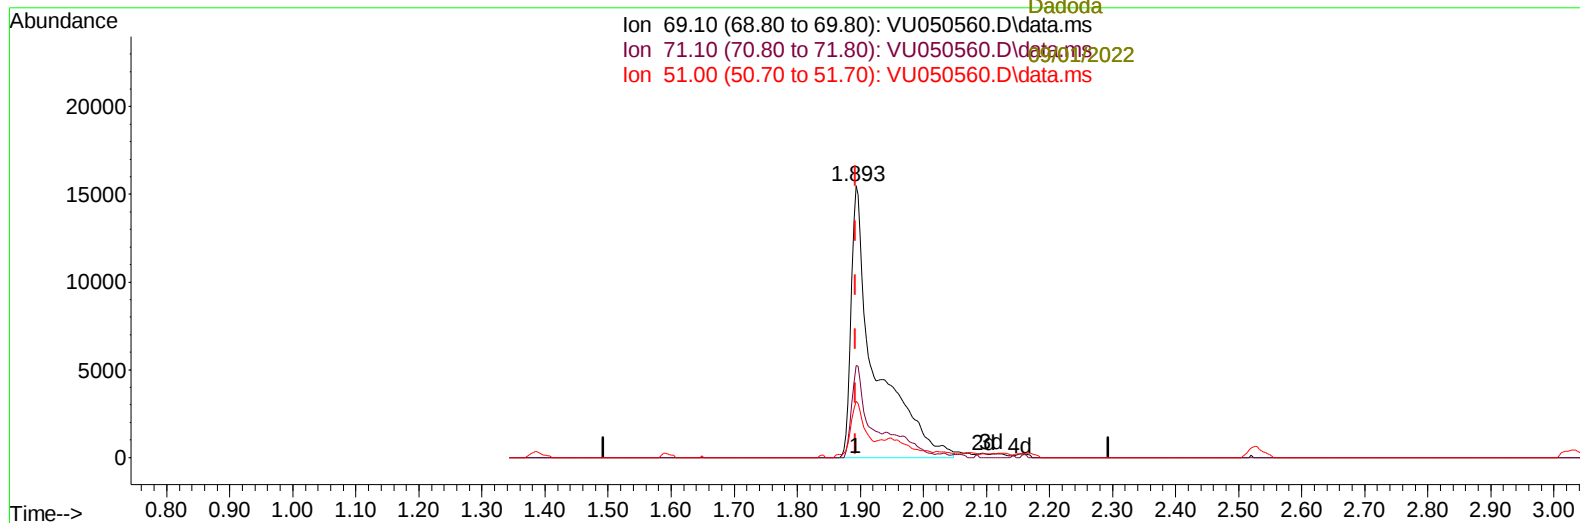

TIC: VU050560.D\data.ms

(7) Chloroethane-d5 (S)

1.893min (-0.000) 26.86 ug/L m

response 41193

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	21.39#
51.00	18.40	12.55#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050560.D
 Acq On : 31 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4363-06ME
 Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW1ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa
 Patel

09/01/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Sep 01 05:19:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----09/01/2022						
Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	256484	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	240484	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	88724	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	71719m	36.459	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	72.920%	
7) Chloroethane-d5	1.893	69	41193m	26.859	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	53.720%#	
11) 1,1-Dichloroethene-d2	2.526	63	118828	35.777	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.560%	
21) 2-Butanone-d5	4.649	46	145675	84.675	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	84.670%	
24) Chloroform-d	5.060	84	179161	46.807	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.620%	
26) 1,2-Dichloroethane-d4	5.700	65	119880	48.216	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.440%	
32) Benzene-d6	5.719	84	370085	49.652	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.300%	
36) 1,2-Dichloropropane-d6	6.690	67	122113	49.204	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	98.400%	
41) Toluene-d8	7.896	98	318049	49.048	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.100%	
43) trans-1,3-Dichloroprop...	8.182	79	45599	45.685	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.380%	
47) 2-Hexanone-d5	8.661	63	89634	99.750	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	99.750%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	163291	42.183	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	84.360%	
66) 1,2-Dichlorobenzene-d4	12.198	152	101396	52.784	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.560%	

Target Compounds						Qvalue
46) Tetrachloroethene	8.552	164	175870	125.411	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050560.D
Acq On : 31 Aug 2022 19:42
Operator : SY/MD
Sample : N4363-06ME
Misc : 5.81g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVW1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:19:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 01 05:15:29 2022
Response via : Initial Calibration

Reviewed By :Krupa
Patel

09/01/2022
Supervised By :Mahesh
Dadoda

09/01/2022

