




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050572.D
 Acq On : 01 Sep 2022 00:25
 Operator : SY/MD
 Sample : N4345-10ME
 Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT0ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:21:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/01/2022

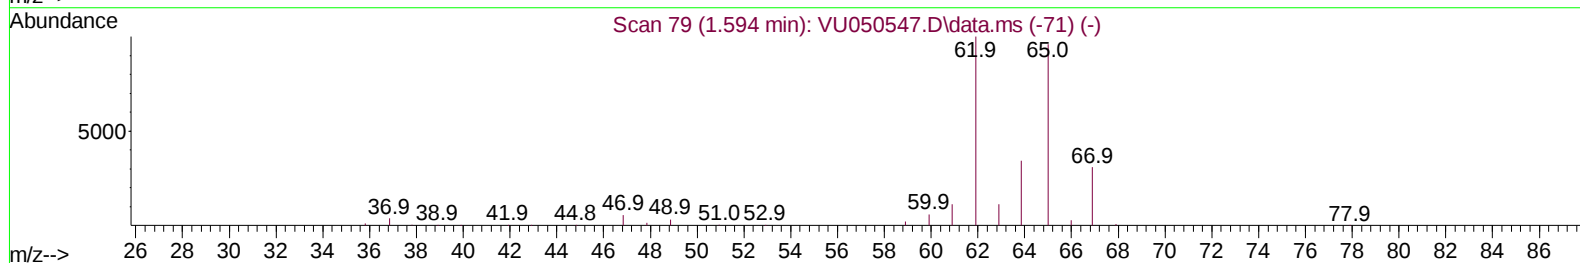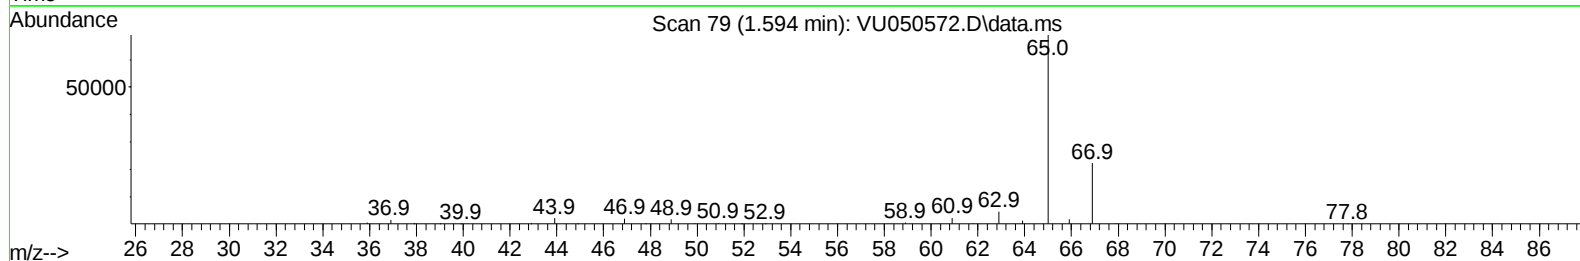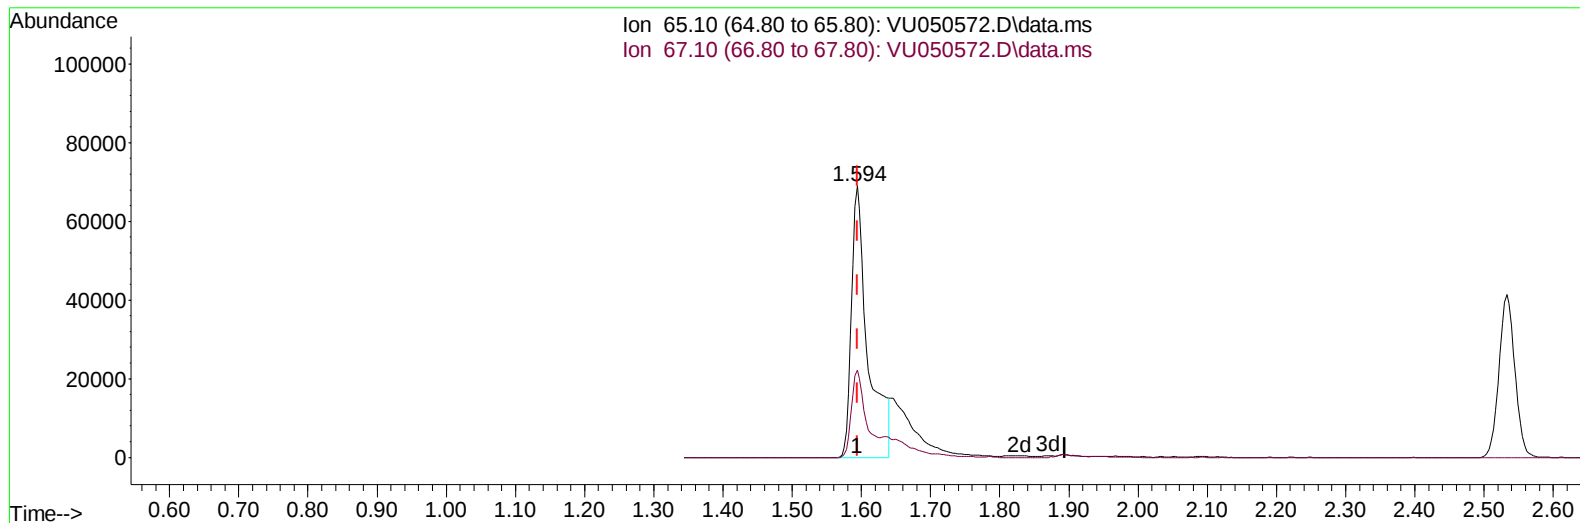

TIC: VU050572.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 39.47 ug/L

response 113315

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	28.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050572.D
 Acq On : 01 Sep 2022 00:25
 Operator : SY/MD
 Sample : N4345-10ME
 Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT0ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:21:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/01/2022

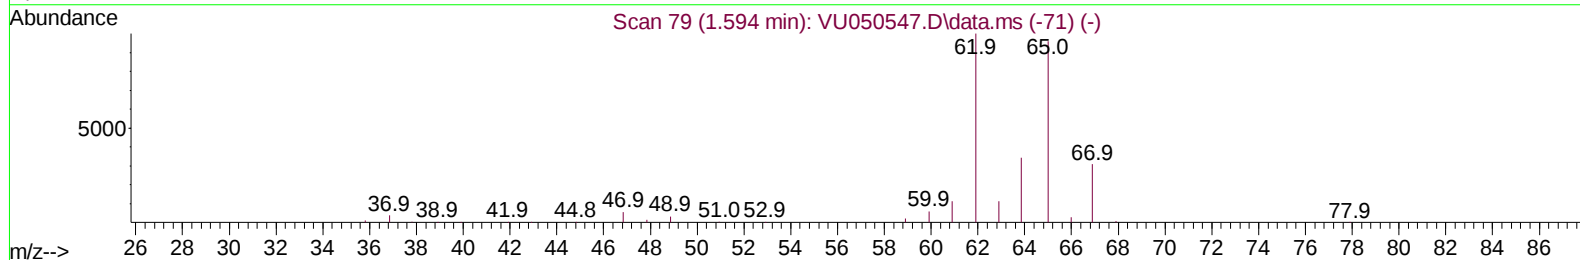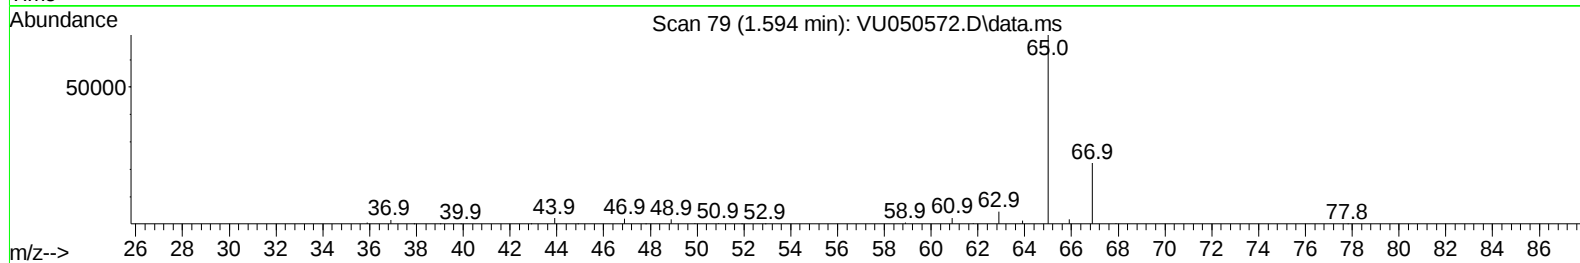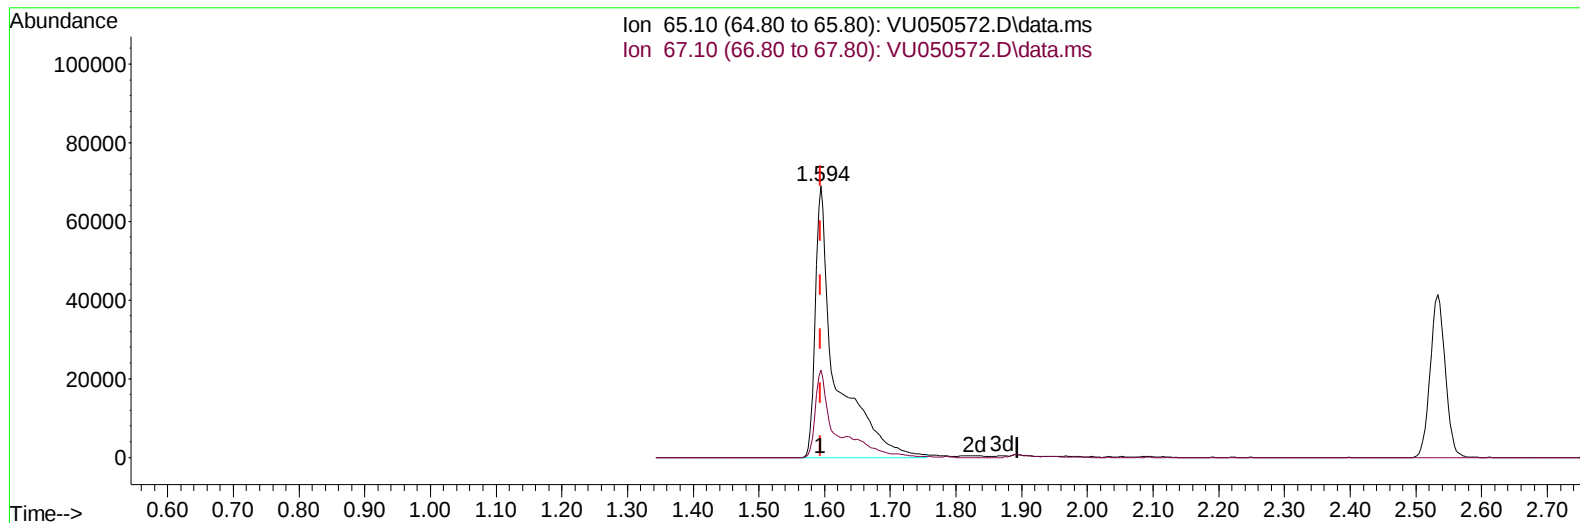

TIC: VU050572.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 52.33 ug/L m

response 150239

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	21.65#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050572.D
 Acq On : 01 Sep 2022 00:25
 Operator : SY/MD
 Sample : N4345-10ME
 Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT0ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:21:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	374327	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	349088	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	99384	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	150239m	52.331	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	104.660%	
7) Chloroethane-d5	1.893	69	60700	27.118	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	54.240%#	
11) 1,1-Dichloroethene-d2	2.533	63	209424	43.204	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.400%	
21) 2-Butanone-d5	4.645	46	281390	112.069	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	112.070%	
24) Chloroform-d	5.060	84	315379	56.456	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	112.920%	
26) 1,2-Dichloroethane-d4	5.700	65	206363	56.871	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.740%	
32) Benzene-d6	5.719	84	669298	61.859	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	123.720%	
36) 1,2-Dichloropropane-d6	6.690	67	224696	62.371	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	124.740%#	
41) Toluene-d8	7.896	98	559810	59.473	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	118.940%	
43) trans-1,3-Dichloroprop...	8.182	79	74352	51.317	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	102.640%	
47) 2-Hexanone-d5	8.661	63	156413	119.912	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	119.910%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	309300	55.043	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	110.080%	
66) 1,2-Dichlorobenzene-d4	12.195	152	135774	63.099	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	126.200%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050572.D
Acq On : 01 Sep 2022 00:25
Operator : SY/MD
Sample : N4345-10ME
Misc : 5.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT0ME

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:21:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 01 05:15:29 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/01/2022

