

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050553.D
 Acq On : 31 Aug 2022 16:56
 Operator : SY/MD
 Sample : N4362-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Quant Time: Sep 01 05:17:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	180248	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	180136	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	64725	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51200	37.036	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	74.080%	
7) Chloroethane-d5	1.903	69	41841	38.820	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	77.640%	
11) 1,1-Dichloroethene-d2	2.562	63	75285	32.254	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	64.500%	
21) 2-Butanone-d5	4.626	46	123056	101.780	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.780%	
24) Chloroform-d	5.060	84	133780	49.734	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.460%	
26) 1,2-Dichloroethane-d4	5.700	65	90280	51.669	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.340%	
32) Benzene-d6	5.726	84	261323	46.806	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.620%	
36) 1,2-Dichloropropane-d6	6.690	67	91249	49.085	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.180%	
41) Toluene-d8	7.899	98	211293	43.501	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.000%	
43) trans-1,3-Dichloroprop...	8.179	79	34048	45.541	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.080%	
47) 2-Hexanone-d5	8.636	63	53811	79.946	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	79.950%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	139961	48.269	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	96.540%	
66) 1,2-Dichlorobenzene-d4	12.195	152	71644	51.125	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.240%	
Target Compounds					Qvalue	
13) Acetone	2.633	43	6697	7.130	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050553.D
Acq On : 31 Aug 2022 16:56
Operator : SY/MD
Sample : N4362-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC2

Quant Time: Sep 01 05:17:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 01 05:15:29 2022
Response via : Initial Calibration

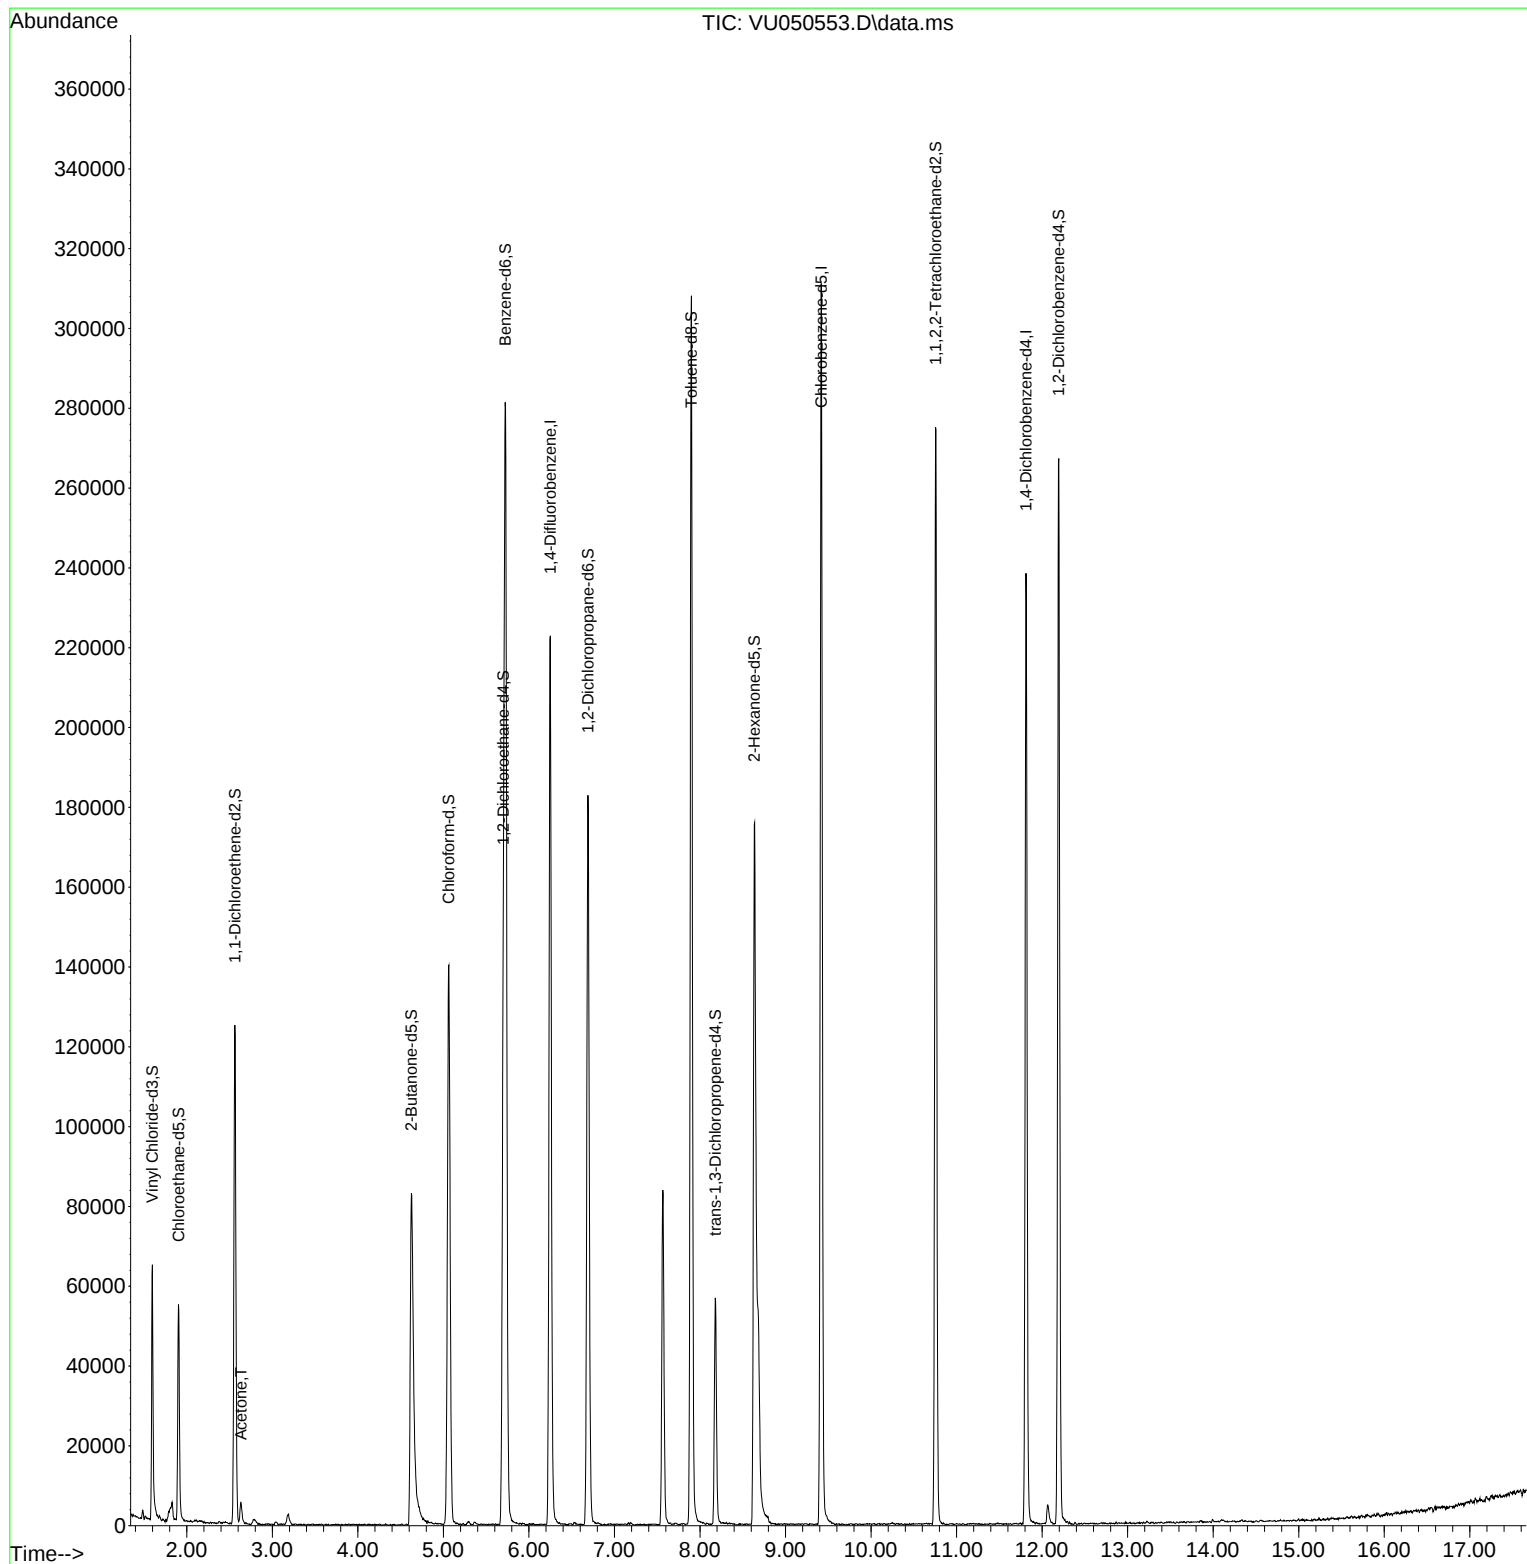

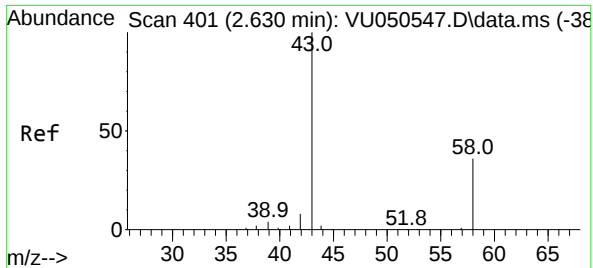

#13
 Acetone
 Concen: 7.130 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU050553.D
 Acq: 31 Aug 2022 16:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Tgt Ion: 43 Resp: 6697
 Ion Ratio Lower Upper
 43 100
 58 37.2 0.0 71.6

