

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050570.D
 Acq On : 31 Aug 2022 23:38
 Operator : SY/MD
 Sample : N4362-07ME
 Misc : 5.02g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB8ME

Quant Time: Sep 01 05:21:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 01 05:15:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	593676	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	509912	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	166374	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	199173	43.743	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.480%
7) Chloroethane-d5	1.890	69	81398	22.929	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	45.860%#
11) 1,1-Dichloroethene-d2	2.536	63	274692	35.731	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.460%
21) 2-Butanone-d5	4.639	46	360877	90.623	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.620%
24) Chloroform-d	5.060	84	410186	46.298	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.697	65	266966	46.389	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.780%
32) Benzene-d6	5.719	84	869535	55.019	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.040%
36) 1,2-Dichloropropane-d6	6.687	67	291344	55.365	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.720%
41) Toluene-d8	7.896	98	751951	54.690	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.380%
43) trans-1,3-Dichloroprop...	8.182	79	84836	40.086	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.180%
47) 2-Hexanone-d5	8.655	63	177750	93.291	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.290%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	351890	42.872	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.740%
66) 1,2-Dichlorobenzene-d4	12.195	152	196732	54.615	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.240%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	8.552	164	21443	7.211	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050570.D
Acq On : 31 Aug 2022 23:38
Operator : SY/MD
Sample : N4362-07ME
Misc : 5.02g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FB8ME


Quant Time: Sep 01 05:21:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 01 05:15:29 2022
Response via : Initial Calibration

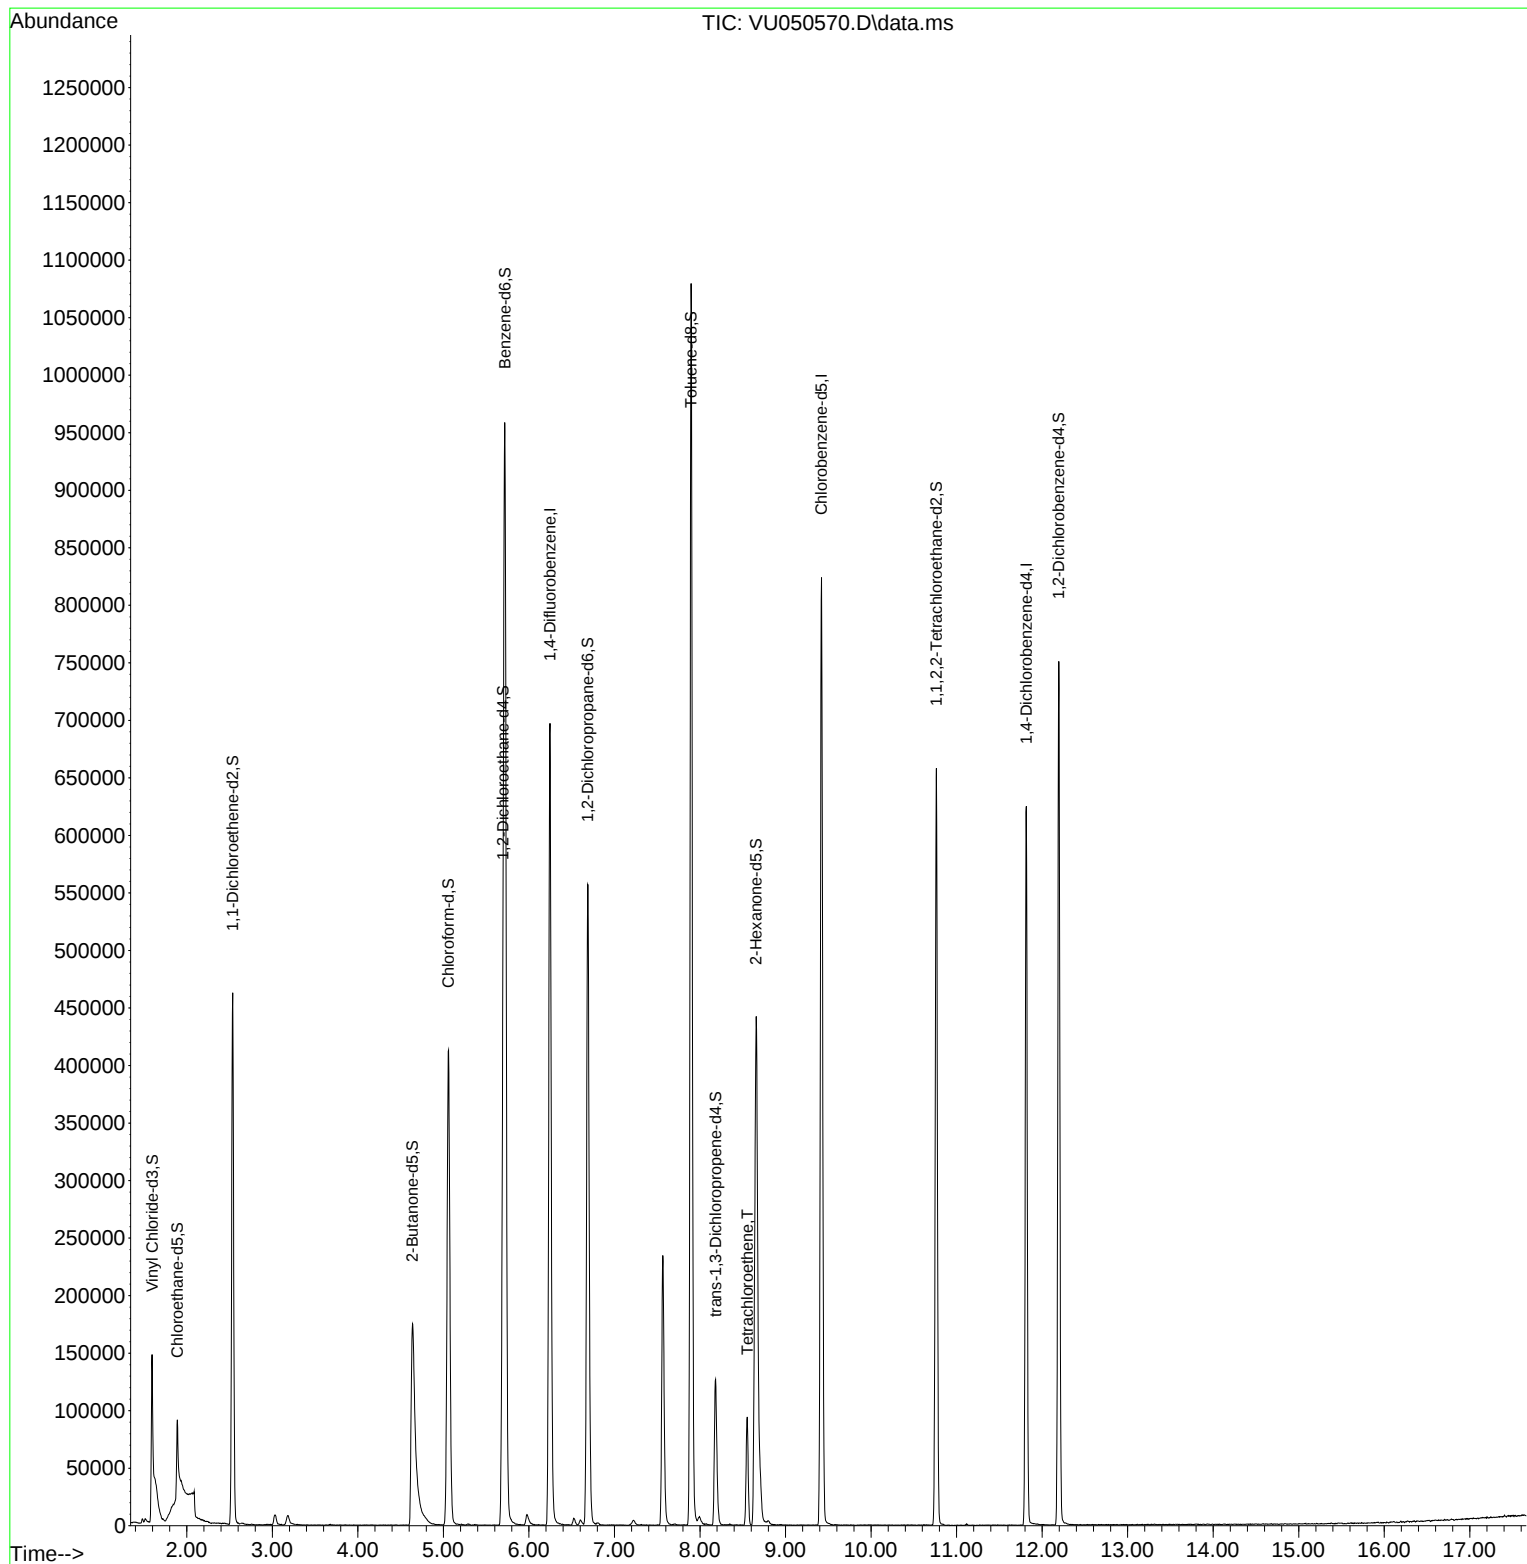

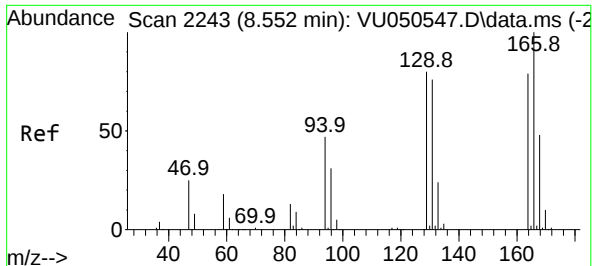

#46
Tetrachloroethene
Concen: 7.211 ug/L
RT: 8.552 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU050570.D
Acq: 31 Aug 2022 23:38

Instrument :
MSVOA_U
ClientSampleId :
C0FB8ME

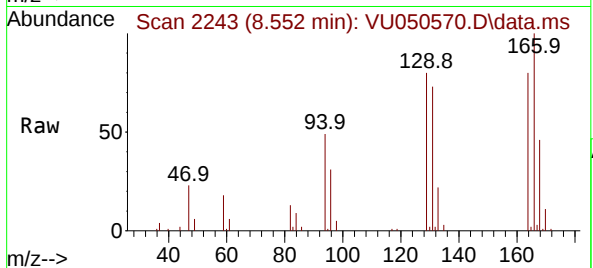

Tgt	Ion:164	Resp:	21443
Ion	Ratio	Lower	Upper
164	100		
129	100.0	67.5	125.3
131	91.9	63.8	118.4
166	125.1	87.2	161.9

