

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050549.D
 Acq On : 31 Aug 2022 15:07
 Operator : SY/MD
 Sample : VU0831WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M

Title : VOC Analysis

Signal : TIC: VU050549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rVB3	2536	2542	0.16%	0.023%
2	1.517	50	55	60	rBV3	2365	3151	0.20%	0.028%
3	1.597	72	80	101	rBV	177847	229398	14.60%	2.055%
4	1.906	167	176	191	rVB	152975	207954	13.23%	1.863%
5	2.562	368	380	396	rBV	306053	496287	31.58%	4.446%
6	2.787	446	450	459	rVB3	995	1161	0.07%	0.010%
7	2.848	464	469	472	rBV	344	320	0.02%	0.003%
8	2.919	485	491	495	rBV2	410	437	0.03%	0.004%
9	2.970	504	507	508	rBV	308	181	0.01%	0.002%
10	2.999	512	516	521	rBV3	270	259	0.02%	0.002%
11	3.044	521	530	539	rVB2	2681	5057	0.32%	0.045%
12	3.086	539	543	548	rBV2	260	276	0.02%	0.002%
13	3.147	559	562	565	rBV2	344	303	0.02%	0.003%
14	3.182	565	573	589	rVB3	3315	7263	0.46%	0.065%
15	3.356	621	627	632	rBV4	1008	1239	0.08%	0.011%
16	3.626	709	711	716	rVB2	372	237	0.02%	0.002%
17	3.793	760	763	767	rBV	314	218	0.01%	0.002%
18	4.012	828	831	835	rVB2	291	219	0.01%	0.002%
19	4.259	904	908	914	rBV2	155	177	0.01%	0.002%
20	4.565	996	1003	1010	rBV2	322	513	0.03%	0.005%
21	4.629	1010	1023	1060	rBV	145702	418001	26.60%	3.744%
22	4.880	1099	1101	1107	rBV3	266	251	0.02%	0.002%
23	5.063	1142	1158	1187	rBV	280559	618767	39.37%	5.543%
24	5.234	1209	1211	1215	rVB2	414	270	0.02%	0.002%
25	5.292	1220	1229	1230	rBV4	972	1324	0.08%	0.012%
26	5.365	1248	1252	1253	rBV3	707	478	0.03%	0.004%
27	5.378	1254	1256	1269	rVB5	1159	1671	0.11%	0.015%
28	5.433	1269	1273	1275	rBV2	303	229	0.01%	0.002%
29	5.523	1296	1301	1305	rBV2	626	598	0.04%	0.005%
30	5.726	1342	1364	1392	rBV2	582639	1571476	100.00%	14.077%
31	6.015	1450	1454	1457	rBV3	424	253	0.02%	0.002%
32	6.108	1479	1483	1485	rBV2	230	200	0.01%	0.002%
33	6.198	1507	1511	1512	rBV	259	209	0.01%	0.002%
34	6.250	1512	1527	1556	rVV	438319	839798	53.44%	7.523%
35	6.533	1605	1615	1626	rVB7	1924	3743	0.24%	0.034%
36	6.690	1649	1664	1687	rBV	370755	726764	46.25%	6.510%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050549.D
 Acq On : 31 Aug 2022 15:07
 Operator : SY/MD
 Sample : VU0831WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.835	1707	1709	1713	rVB	594	345	0.02%	0.003%
38	6.854	1713	1715	1720	rVB	282	187	0.01%	0.002%
39	6.980	1749	1754	1757	rVV3	228	261	0.02%	0.002%
40	7.025	1761	1768	1771	rVB2	342	308	0.02%	0.003%
41	7.044	1771	1774	1780	rBV2	269	309	0.02%	0.003%
42	7.189	1814	1819	1822	rBV2	529	442	0.03%	0.004%
43	7.565	1923	1936	1959	rBV	162413	295209	18.79%	2.644%
44	7.716	1981	1983	1988	rVB2	409	244	0.02%	0.002%
45	7.806	2003	2011	2014	rBV4	784	828	0.05%	0.007%
46	7.848	2019	2024	2026	rBV2	298	307	0.02%	0.003%
47	7.899	2026	2040	2074	rBV	668274	1162410	73.97%	10.413%
48	8.134	2108	2113	2116	rVB3	268	266	0.02%	0.002%
49	8.179	2116	2127	2152	rBV	111361	196746	12.52%	1.762%
50	8.362	2181	2184	2187	rVB2	435	259	0.02%	0.002%
51	8.407	2192	2198	2202	rVB5	864	986	0.06%	0.009%
52	8.475	2217	2219	2222	rBV	366	228	0.01%	0.002%
53	8.520	2229	2233	2239	rBV2	335	403	0.03%	0.004%
54	8.552	2239	2243	2249	rVB2	985	1112	0.07%	0.010%
55	8.639	2257	2270	2325	rBV5	313985	845490	53.80%	7.574%
56	8.886	2344	2347	2351	rVB2	402	267	0.02%	0.002%
57	8.922	2356	2358	2360	rVV2	421	238	0.02%	0.002%
58	8.934	2360	2362	2367	rVB3	411	282	0.02%	0.003%
59	9.079	2404	2407	2414	rBV2	242	250	0.02%	0.002%
60	9.134	2422	2424	2432	rVB	302	291	0.02%	0.003%
61	9.417	2497	2512	2545	rBV	606995	1031492	65.64%	9.240%
62	9.568	2556	2559	2571	rVB5	1330	1929	0.12%	0.017%
63	9.623	2571	2576	2579	rVV3	250	296	0.02%	0.003%
64	9.687	2591	2596	2597	rBV2	701	559	0.04%	0.005%
65	9.745	2611	2614	2618	rBV2	210	183	0.01%	0.002%
66	10.105	2718	2726	2732	rBV5	1369	2323	0.15%	0.021%
67	10.298	2780	2786	2787	rBV	221	207	0.01%	0.002%
68	10.455	2833	2835	2838	rVB	489	215	0.01%	0.002%
69	10.487	2838	2845	2849	rBV3	1067	1252	0.08%	0.011%
70	10.539	2856	2861	2863	rBV2	254	248	0.02%	0.002%
71	10.587	2874	2876	2881	rVB	291	182	0.01%	0.002%
72	10.635	2889	2891	2893	rVV	491	283	0.02%	0.003%
73	10.758	2915	2929	2954	rBV	509172	828801	52.74%	7.424%
74	11.095	3028	3034	3042	rVB4	716	915	0.06%	0.008%
75	11.166	3053	3056	3061	rBV2	313	358	0.02%	0.003%
76	11.217	3069	3072	3077	rBV2	309	234	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050549.D
 Acq On : 31 Aug 2022 15:07
 Operator : SY/MD
 Sample : VU0831WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK175

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	11.330	3103	3107	3111	rBV2	302	259	0.02%	0.002%
78	11.471	3144	3151	3159	rVB4	1186	1560	0.10%	0.014%
79	11.503	3159	3161	3163	rBV	314	197	0.01%	0.002%
80	11.606	3189	3193	3196	rBV2	273	245	0.02%	0.002%
81	11.748	3232	3237	3242	rBV3	1161	1272	0.08%	0.011%
82	11.812	3245	3257	3279	rBV	464541	743968	47.34%	6.664%
83	12.121	3350	3353	3356	rBV	320	286	0.02%	0.003%
84	12.195	3361	3376	3401	rBV	529466	878025	55.87%	7.865%
85	12.513	3472	3475	3477	rBV	331	180	0.01%	0.002%
86	12.626	3507	3510	3515	rBV2	371	405	0.03%	0.004%
87	12.819	3566	3570	3573	rBV2	486	398	0.03%	0.004%
88	12.873	3584	3587	3590	rBV2	399	300	0.02%	0.003%
89	13.076	3646	3650	3652	rBV3	327	278	0.02%	0.002%
90	13.118	3660	3663	3666	rBV2	429	265	0.02%	0.002%
91	13.179	3675	3682	3683	rBV3	349	405	0.03%	0.004%
92	13.227	3691	3697	3701	rBV5	1174	1217	0.08%	0.011%
93	13.272	3706	3711	3717	rBV3	480	562	0.04%	0.005%
94	13.410	3751	3754	3757	rVB	509	333	0.02%	0.003%
95	13.429	3757	3760	3765	rBV3	352	430	0.03%	0.004%
96	13.847	3884	3890	3899	rVB6	2577	3601	0.23%	0.032%
97	13.892	3902	3904	3910	rVB3	404	250	0.02%	0.002%
98	13.982	3930	3932	3936	rBV	326	249	0.02%	0.002%
99	14.095	3960	3967	3978	rBV3	3774	6555	0.42%	0.059%
100	14.339	4037	4043	4051	rVB6	2647	3688	0.23%	0.033%




Sum of corrected areas: 11163297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050549.D
Acq On : 31 Aug 2022 15:07
Operator : SY/MD
Sample : VU0831WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

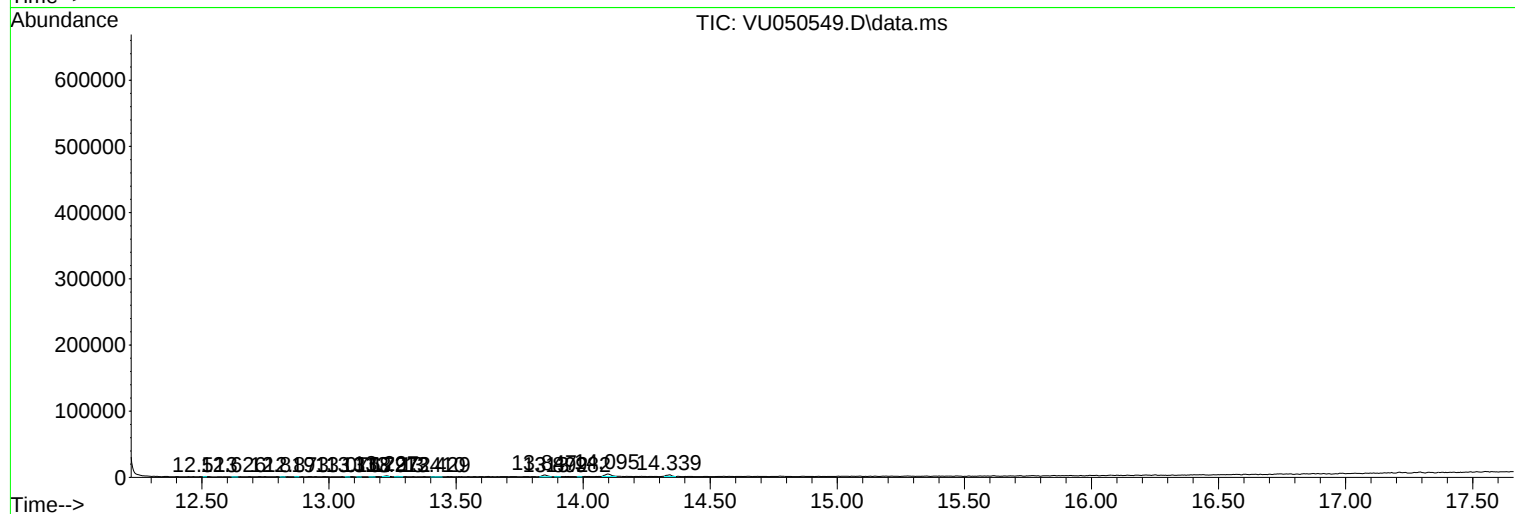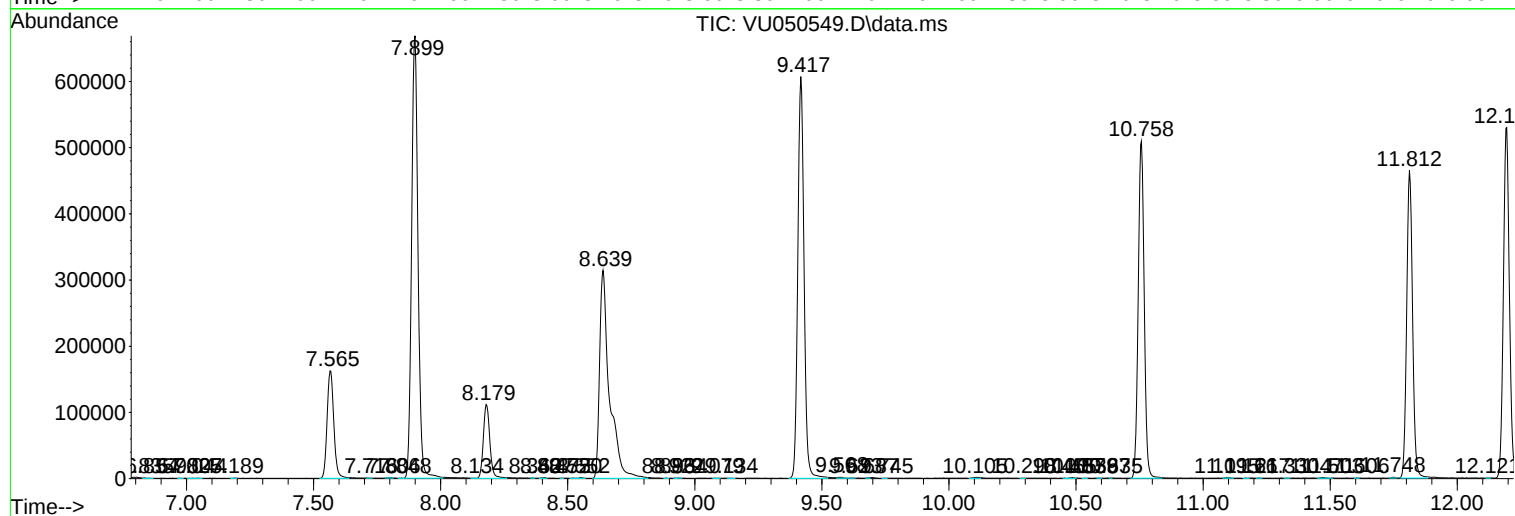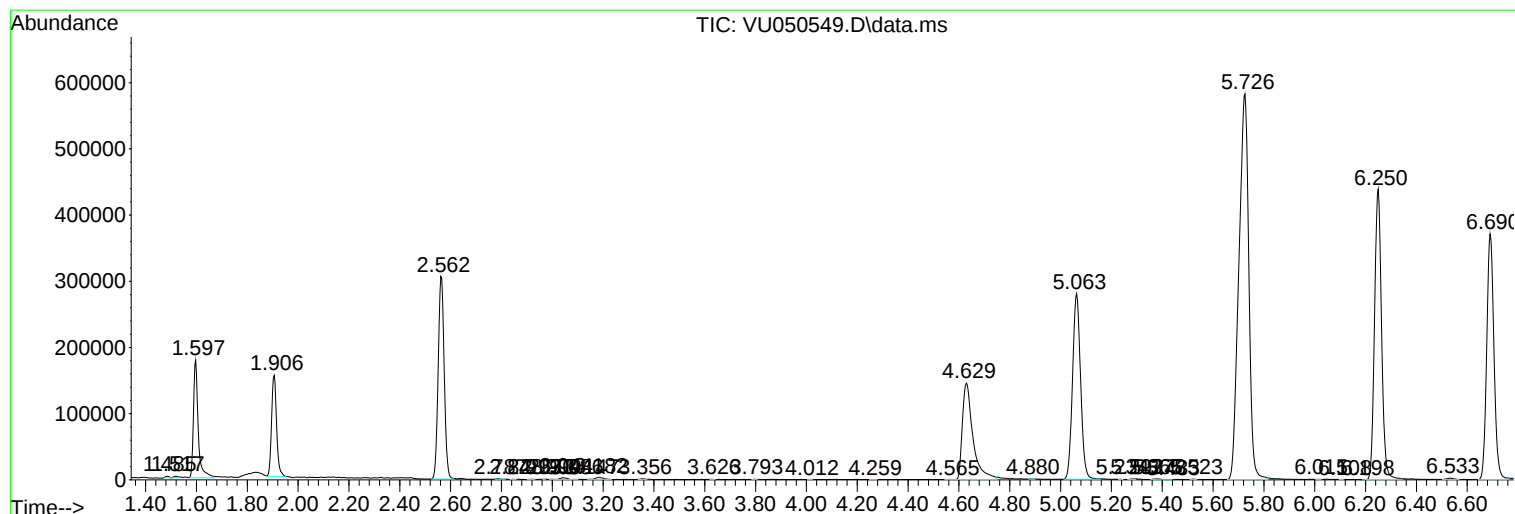

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050549.D
Acq On : 31 Aug 2022 15:07
Operator : SY/MD
Sample : VU0831WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050549.D
Acq On : 31 Aug 2022 15:07
Operator : SY/MD
Sample : VU0831WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK175

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------