

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050550.D
 Acq On : 31 Aug 2022 15:45
 Operator : SY/MD
 Sample : N4440-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	3280	3646	0.25%	0.036%
2	1.597	72	80	99	rBV	159717	197165	13.66%	1.949%
3	1.909	168	177	197	rVB	141013	187961	13.02%	1.858%
4	2.565	367	381	395	rBV	265230	429511	29.76%	4.246%
5	2.633	396	402	415	rVB	5332	9605	0.67%	0.095%
6	2.732	430	433	435	rVB2	322	197	0.01%	0.002%
7	2.771	436	445	447	rVV4	865	863	0.06%	0.009%
8	2.787	447	450	464	rVB4	1314	2151	0.15%	0.021%
9	2.861	470	473	476	rBV2	253	158	0.01%	0.002%
10	3.179	566	572	573	rBV4	788	757	0.05%	0.007%
11	3.449	652	656	660	rVV3	230	205	0.01%	0.002%
12	3.501	668	672	674	rBV	343	237	0.02%	0.002%
13	3.588	688	699	711	rBV4	2085	4173	0.29%	0.041%
14	3.636	711	714	717	rBV3	266	181	0.01%	0.002%
15	3.771	754	756	759	rVB	312	155	0.01%	0.002%
16	3.793	759	763	766	rBV2	201	189	0.01%	0.002%
17	3.887	787	792	797	rBV2	222	221	0.02%	0.002%
18	3.938	805	808	812	rBV2	215	220	0.02%	0.002%
19	4.015	829	832	838	rBV2	265	322	0.02%	0.003%
20	4.064	842	847	852	rVB2	275	382	0.03%	0.004%
21	4.105	852	860	862	rBV2	395	543	0.04%	0.005%
22	4.186	879	885	888	rBV2	226	231	0.02%	0.002%
23	4.388	944	948	951	rBV2	260	221	0.02%	0.002%
24	4.430	955	961	963	rBV2	392	354	0.02%	0.003%
25	4.446	963	966	972	rVB5	450	522	0.04%	0.005%
26	4.568	998	1004	1007	rBV2	363	442	0.03%	0.004%
27	4.626	1009	1022	1045	rBV2	142381	388602	26.92%	3.842%
28	5.064	1139	1158	1181	rBV	266051	585899	40.59%	5.792%
29	5.289	1222	1228	1229	rBV5	840	750	0.05%	0.007%
30	5.369	1248	1253	1255	rBV3	384	402	0.03%	0.004%
31	5.417	1264	1268	1275	rVB2	216	218	0.02%	0.002%
32	5.726	1342	1364	1387	rBV2	534146	1443475	100.00%	14.270%
33	5.964	1435	1438	1441	rBV2	305	224	0.02%	0.002%
34	6.089	1474	1477	1481	rVB	364	247	0.02%	0.002%
35	6.115	1481	1485	1488	rBV2	322	284	0.02%	0.003%
36	6.250	1512	1527	1552	rBV	388987	744154	51.55%	7.357%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050550.D
 Acq On : 31 Aug 2022 15:45
 Operator : SY/MD
 Sample : N4440-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.498	1601	1604	1607	rVB2	273	167	0.01%	0.002%
38	6.533	1607	1615	1623	rVV4	1114	1879	0.13%	0.019%
39	6.565	1623	1625	1627	rVV2	355	157	0.01%	0.002%
40	6.584	1627	1631	1635	rVB2	250	181	0.01%	0.002%
41	6.690	1650	1664	1686	rBV	338522	674258	46.71%	6.666%
42	6.803	1696	1699	1701	rBV3	625	396	0.03%	0.004%
43	6.874	1718	1721	1723	rBV	350	204	0.01%	0.002%
44	6.973	1750	1752	1758	rVB2	326	243	0.02%	0.002%
45	7.031	1767	1770	1774	rBV2	279	157	0.01%	0.002%
46	7.099	1788	1791	1794	rBV2	261	222	0.02%	0.002%
47	7.134	1798	1802	1805	rVV2	465	387	0.03%	0.004%
48	7.173	1810	1814	1817	rVB3	281	213	0.01%	0.002%
49	7.195	1817	1821	1829	rVB4	456	556	0.04%	0.005%
50	7.244	1829	1836	1840	rBV2	319	420	0.03%	0.004%
51	7.356	1864	1871	1873	rBV2	149	183	0.01%	0.002%
52	7.568	1924	1937	1956	rBV	153335	274166	18.99%	2.710%
53	7.710	1979	1981	1984	rVB2	434	199	0.01%	0.002%
54	7.729	1984	1987	1992	rVB3	285	211	0.01%	0.002%
55	7.797	2002	2008	2020	rBV3	2389	3703	0.26%	0.037%
56	7.899	2025	2040	2066	rBV	591398	1029235	71.30%	10.175%
57	8.182	2116	2128	2150	rBV	106027	181979	12.61%	1.799%
58	8.388	2188	2192	2194	rBV2	282	225	0.02%	0.002%
59	8.456	2209	2213	2218	rVB3	372	391	0.03%	0.004%
60	8.485	2218	2222	2225	rBV2	341	302	0.02%	0.003%
61	8.526	2231	2235	2237	rBV2	290	198	0.01%	0.002%
62	8.542	2237	2240	2244	rVB	419	211	0.01%	0.002%
63	8.588	2250	2254	2256	rBV	239	153	0.01%	0.002%
64	8.639	2256	2270	2306	rBV4	306536	803083	55.64%	7.939%
65	9.083	2406	2408	2413	rBV2	232	232	0.02%	0.002%
66	9.208	2445	2447	2454	rVB	331	328	0.02%	0.003%
67	9.253	2454	2461	2466	rBV2	345	466	0.03%	0.005%
68	9.417	2499	2512	2536	rBV	548723	925925	64.15%	9.154%
69	10.060	2707	2712	2714	rBV	223	211	0.01%	0.002%
70	10.086	2716	2720	2721	rBV2	563	393	0.03%	0.004%
71	10.186	2748	2751	2756	rVB2	285	233	0.02%	0.002%
72	10.247	2761	2770	2780	rVV3	900	1516	0.11%	0.015%
73	10.349	2799	2802	2804	rBV3	421	250	0.02%	0.002%
74	10.491	2841	2846	2849	rBV3	403	388	0.03%	0.004%
75	10.517	2850	2854	2858	rBV2	227	214	0.01%	0.002%
76	10.758	2915	2929	2954	rBV	428689	710247	49.20%	7.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050550.D
 Acq On : 31 Aug 2022 15:45
 Operator : SY/MD
 Sample : N4440-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	11.124	3038	3043	3046	rBV2	249	319	0.02%	0.003%
78	11.272	3083	3089	3094	rBV2	311	347	0.02%	0.003%
79	11.369	3116	3119	3122	rBV	249	168	0.01%	0.002%
80	11.488	3151	3156	3163	rVB4	977	1286	0.09%	0.013%
81	11.552	3172	3176	3179	rBV2	237	228	0.02%	0.002%
82	11.642	3201	3204	3211	rVB3	418	293	0.02%	0.003%
83	11.745	3233	3236	3239	rBV3	549	379	0.03%	0.004%
84	11.812	3245	3257	3282	rBV	410201	671830	46.54%	6.642%
85	11.964	3301	3304	3309	rBV3	351	348	0.02%	0.003%
86	12.070	3330	3337	3352	rVB5	4035	7200	0.50%	0.071%
87	12.195	3363	3376	3401	rBV	491910	802852	55.62%	7.937%
88	12.417	3442	3445	3448	rBV3	452	399	0.03%	0.004%
89	12.529	3476	3480	3482	rBV	332	272	0.02%	0.003%
90	12.555	3486	3488	3491	rVB	403	239	0.02%	0.002%
91	12.671	3522	3524	3530	rVB3	542	470	0.03%	0.005%
92	12.703	3530	3534	3536	rBV	354	230	0.02%	0.002%
93	12.809	3564	3567	3569	rBV2	307	180	0.01%	0.002%
94	13.150	3671	3673	3680	rVB2	281	242	0.02%	0.002%
95	13.230	3692	3698	3704	rBV4	916	1199	0.08%	0.012%
96	13.652	3828	3829	3834	rVB	297	231	0.02%	0.002%
97	13.761	3861	3863	3867	rBV2	310	167	0.01%	0.002%
98	13.851	3884	3891	3898	rVV4	1576	2191	0.15%	0.022%
99	14.095	3961	3967	3970	rBV2	2537	2671	0.19%	0.026%
100	14.340	4035	4043	4051	rVB5	1667	2419	0.17%	0.024%




Sum of corrected areas: 10115109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050550.D
Acq On : 31 Aug 2022 15:45
Operator : SY/MD
Sample : N4440-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

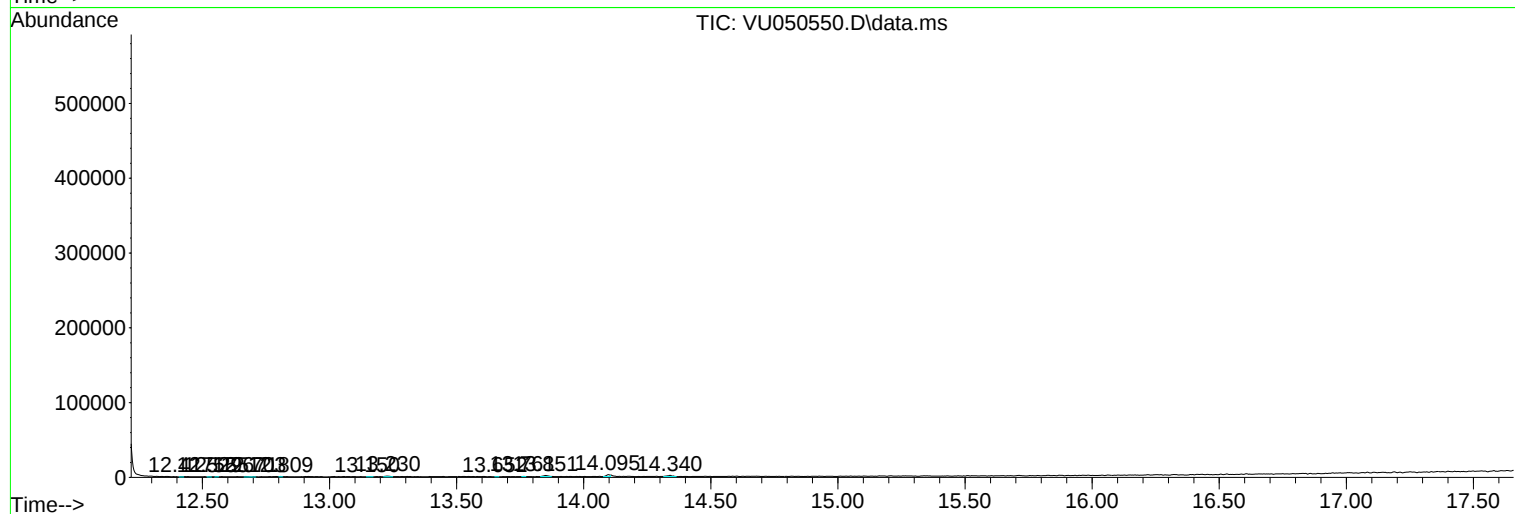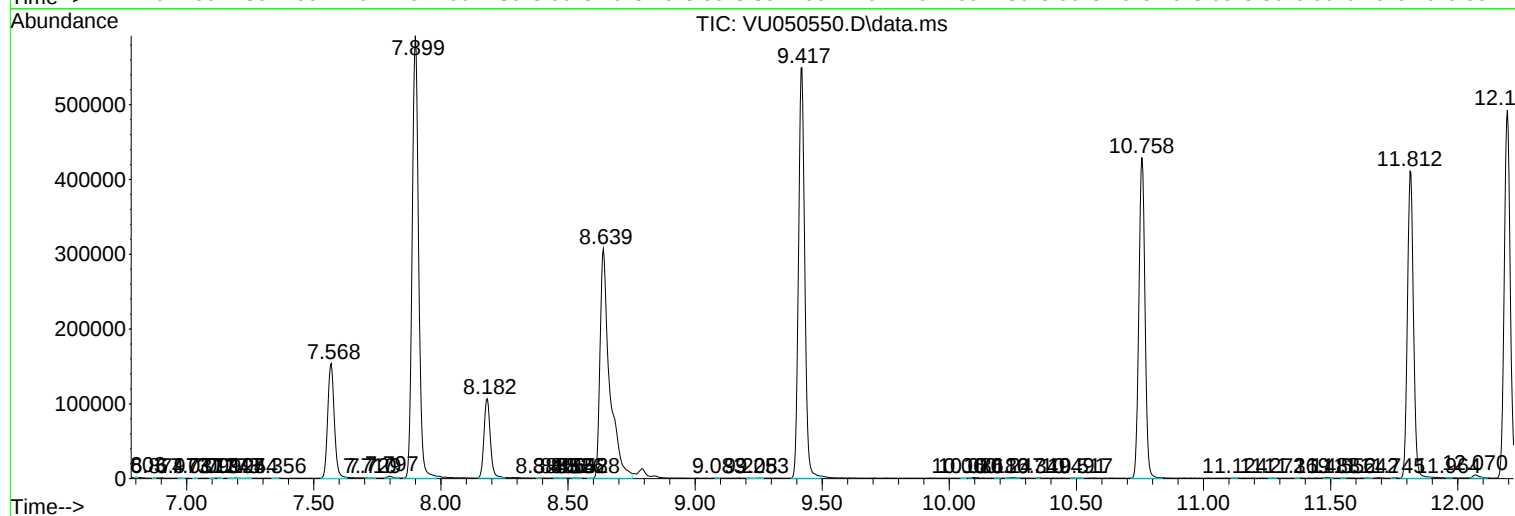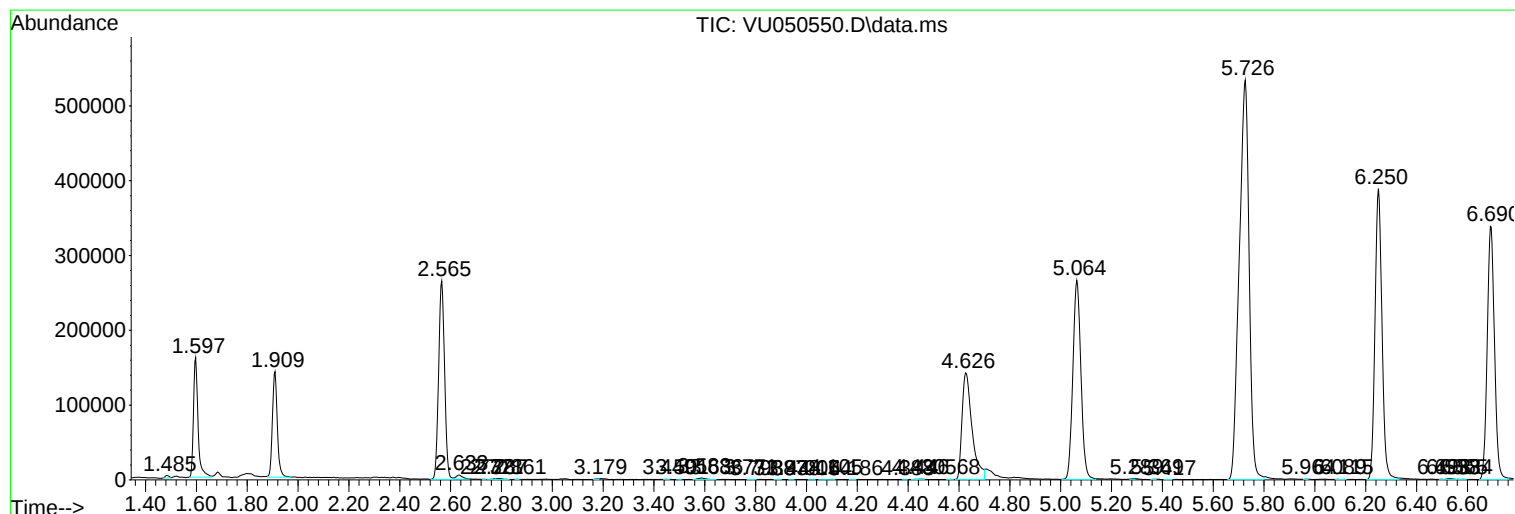

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050550.D
Acq On : 31 Aug 2022 15:45
Operator : SY/MD
Sample : N4440-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050550.D
Acq On : 31 Aug 2022 15:45
Operator : SY/MD
Sample : N4440-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc