

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050551.D
 Acq On : 31 Aug 2022 16:09
 Operator : SY/MD
 Sample : N4440-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV3	2762	2722	0.22%	0.032%
2	1.597	72	80	102	rBV	121258	154954	12.48%	1.809%
3	1.903	167	175	193	rVB	114037	154575	12.45%	1.804%
4	2.562	368	380	394	rBV	214717	343369	27.66%	4.008%
5	2.790	445	451	459	rVB3	736	990	0.08%	0.012%
6	2.906	483	487	490	rBV3	315	233	0.02%	0.003%
7	2.922	490	492	496	rVB2	307	222	0.02%	0.003%
8	2.954	497	502	505	rBV3	568	667	0.05%	0.008%
9	3.041	523	529	538	rVB3	1068	1731	0.14%	0.020%
10	3.128	552	556	559	rBV2	218	180	0.01%	0.002%
11	3.147	559	562	565	rBV2	233	167	0.01%	0.002%
12	3.189	565	575	578	rBV4	1057	1685	0.14%	0.020%
13	3.273	596	601	603	rBV2	209	175	0.01%	0.002%
14	3.295	606	608	613	rVV	283	204	0.02%	0.002%
15	3.363	625	629	630	rBV2	260	179	0.01%	0.002%
16	3.562	689	691	698	rVB2	329	299	0.02%	0.003%
17	3.604	698	704	707	rBV2	170	218	0.02%	0.003%
18	3.768	751	755	761	rBV	270	266	0.02%	0.003%
19	3.797	761	764	774	rVB2	157	218	0.02%	0.003%
20	4.051	838	843	846	rBV2	219	200	0.02%	0.002%
21	4.160	872	877	880	rBV2	254	314	0.03%	0.004%
22	4.318	923	926	928	rBV	248	172	0.01%	0.002%
23	4.453	962	968	970	rBV2	286	260	0.02%	0.003%
24	4.575	1002	1006	1009	rBV2	187	203	0.02%	0.002%
25	4.626	1009	1022	1044	rBV	136230	365052	29.41%	4.261%
26	4.961	1124	1126	1130	rVB	407	221	0.02%	0.003%
27	5.063	1141	1158	1178	rBV	231382	512165	41.26%	5.978%
28	5.186	1191	1196	1198	rVB3	314	224	0.02%	0.003%
29	5.289	1220	1228	1233	rBV3	1392	2348	0.19%	0.027%
30	5.369	1248	1253	1254	rBV	617	390	0.03%	0.005%
31	5.433	1269	1273	1281	rBV2	180	279	0.02%	0.003%
32	5.597	1321	1324	1329	rVB2	189	169	0.01%	0.002%
33	5.723	1341	1363	1389	rBV2	455267	1241429	100.00%	14.490%
34	5.977	1440	1442	1451	rVB3	609	436	0.04%	0.005%
35	6.057	1463	1467	1471	rBV3	321	262	0.02%	0.003%
36	6.108	1477	1483	1485	rBV2	416	381	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050551.D
 Acq On : 31 Aug 2022 16:09
 Operator : SY/MD
 Sample : N4440-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.121	1485	1487	1491	rVV	369	275	0.02%	0.003%
38	6.250	1512	1527	1558	rBV	320915	625555	50.39%	7.301%
39	6.526	1608	1613	1617	rBV3	1142	1262	0.10%	0.015%
40	6.594	1633	1634	1640	rVB3	297	162	0.01%	0.002%
41	6.690	1650	1664	1691	rVV	299558	584932	47.12%	6.827%
42	6.797	1694	1697	1706	rVV5	1272	1881	0.15%	0.022%
43	6.835	1706	1709	1714	rVB3	501	368	0.03%	0.004%
44	6.887	1721	1725	1732	rBV4	635	698	0.06%	0.008%
45	6.938	1737	1741	1743	rBV2	234	168	0.01%	0.002%
46	6.986	1753	1756	1759	rBV	280	211	0.02%	0.002%
47	7.189	1813	1819	1822	rBV	447	611	0.05%	0.007%
48	7.391	1877	1882	1884	rBV2	288	262	0.02%	0.003%
49	7.449	1895	1900	1904	rBV2	208	190	0.02%	0.002%
50	7.565	1923	1936	1957	rBV	130777	236301	19.03%	2.758%
51	7.719	1981	1984	1987	rBV2	276	209	0.02%	0.002%
52	7.793	1997	2007	2020	rBV5	2769	4919	0.40%	0.057%
53	7.848	2020	2024	2026	rBV2	303	216	0.02%	0.003%
54	7.896	2026	2039	2064	rBV	486475	858008	69.11%	10.015%
55	8.179	2116	2127	2147	rBV	90303	152189	12.26%	1.776%
56	8.247	2147	2148	2155	rVB4	598	494	0.04%	0.006%
57	8.327	2170	2173	2175	rVB	440	232	0.02%	0.003%
58	8.350	2175	2180	2187	rVB3	521	643	0.05%	0.008%
59	8.395	2192	2194	2198	rBV2	186	170	0.01%	0.002%
60	8.488	2220	2223	2225	rBV	281	199	0.02%	0.002%
61	8.636	2257	2269	2307	rBV4	289539	749350	60.36%	8.746%
62	8.787	2312	2316	2327	rVB3	13891	20716	1.67%	0.242%
63	8.941	2363	2364	2370	rVB	290	166	0.01%	0.002%
64	9.221	2447	2451	2457	rBV3	239	258	0.02%	0.003%
65	9.253	2458	2461	2465	rBV	211	168	0.01%	0.002%
66	9.311	2476	2479	2481	rBV	273	196	0.02%	0.002%
67	9.330	2481	2485	2489	rBV	509	403	0.03%	0.005%
68	9.417	2498	2512	2533	rBV	468863	777563	62.63%	9.076%
69	9.697	2594	2599	2600	rBV2	409	315	0.03%	0.004%
70	9.848	2643	2646	2649	rBV2	217	161	0.01%	0.002%
71	10.041	2700	2706	2711	rBV	354	364	0.03%	0.004%
72	10.086	2712	2720	2732	rVV2	4068	7176	0.58%	0.084%
73	10.221	2754	2762	2763	rBV3	422	497	0.04%	0.006%
74	10.237	2763	2767	2777	rVV3	837	1437	0.12%	0.017%
75	10.349	2797	2802	2807	rVV3	793	1050	0.08%	0.012%
76	10.565	2864	2869	2873	rBV	449	402	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050551.D
 Acq On : 31 Aug 2022 16:09
 Operator : SY/MD
 Sample : N4440-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2952	rBV	334981	541826	43.65%	6.324%
78	11.060	3021	3023	3027	rBV2	230	160	0.01%	0.002%
79	11.111	3036	3039	3041	rBV2	392	214	0.02%	0.002%
80	11.343	3108	3111	3118	rVB2	309	370	0.03%	0.004%
81	11.484	3149	3155	3159	rBV3	812	1103	0.09%	0.013%
82	11.574	3180	3183	3186	rBV2	363	214	0.02%	0.002%
83	11.693	3216	3220	3228	rVB4	812	905	0.07%	0.011%
84	11.742	3232	3235	3237	rBV2	486	300	0.02%	0.004%
85	11.812	3244	3257	3280	rBV	318965	511207	41.18%	5.967%
86	12.070	3327	3337	3348	rBV5	3772	7208	0.58%	0.084%
87	12.134	3354	3357	3359	rBV	264	169	0.01%	0.002%
88	12.195	3363	3376	3399	rBV	414884	681343	54.88%	7.953%
89	12.365	3427	3429	3432	rVB3	310	170	0.01%	0.002%
90	12.549	3483	3486	3489	rBV3	477	372	0.03%	0.004%
91	12.623	3505	3509	3512	rBV3	334	339	0.03%	0.004%
92	12.828	3570	3573	3577	rBV	321	284	0.02%	0.003%
93	12.896	3590	3594	3603	rVB5	1175	1416	0.11%	0.017%
94	13.018	3629	3632	3635	rBV	347	276	0.02%	0.003%
95	13.179	3679	3682	3685	rBV	320	300	0.02%	0.004%
96	13.330	3727	3729	3736	rVB2	279	278	0.02%	0.003%
97	13.629	3818	3822	3823	rBV2	430	305	0.02%	0.004%
98	14.028	3944	3946	3952	rBV2	319	177	0.01%	0.002%
99	14.545	4104	4107	4109	rBV3	323	245	0.02%	0.003%
100	15.095	4276	4278	4283	rVB2	548	423	0.03%	0.005%




Sum of corrected areas: 8567540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050551.D
Acq On : 31 Aug 2022 16:09
Operator : SY/MD
Sample : N4440-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

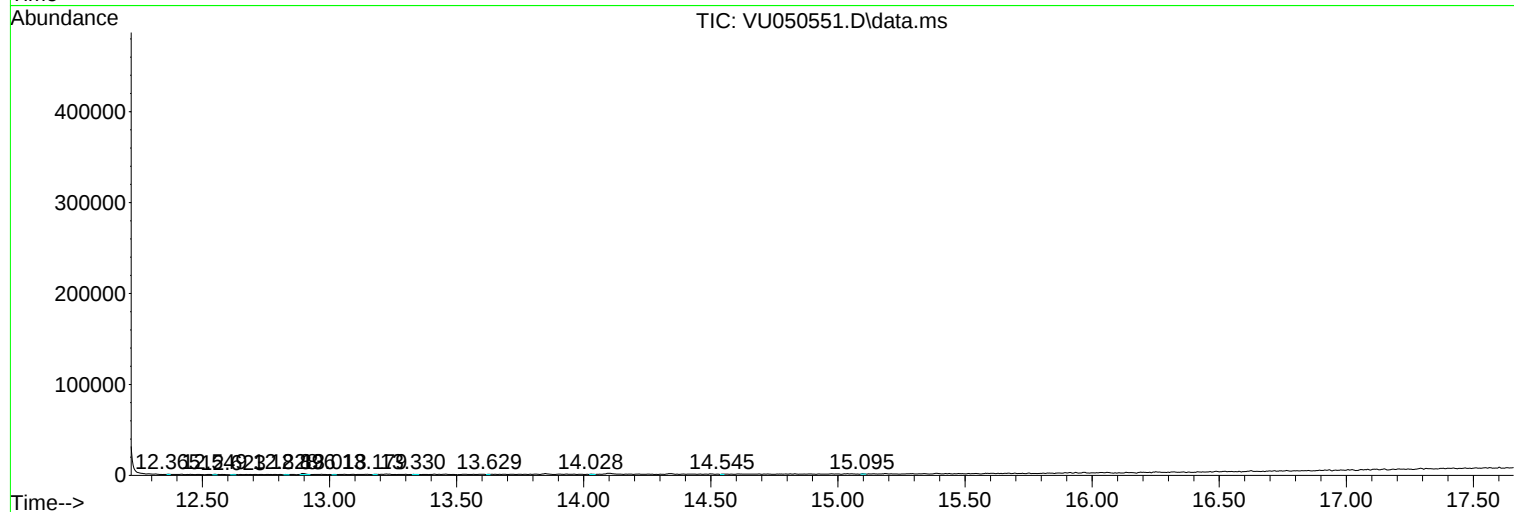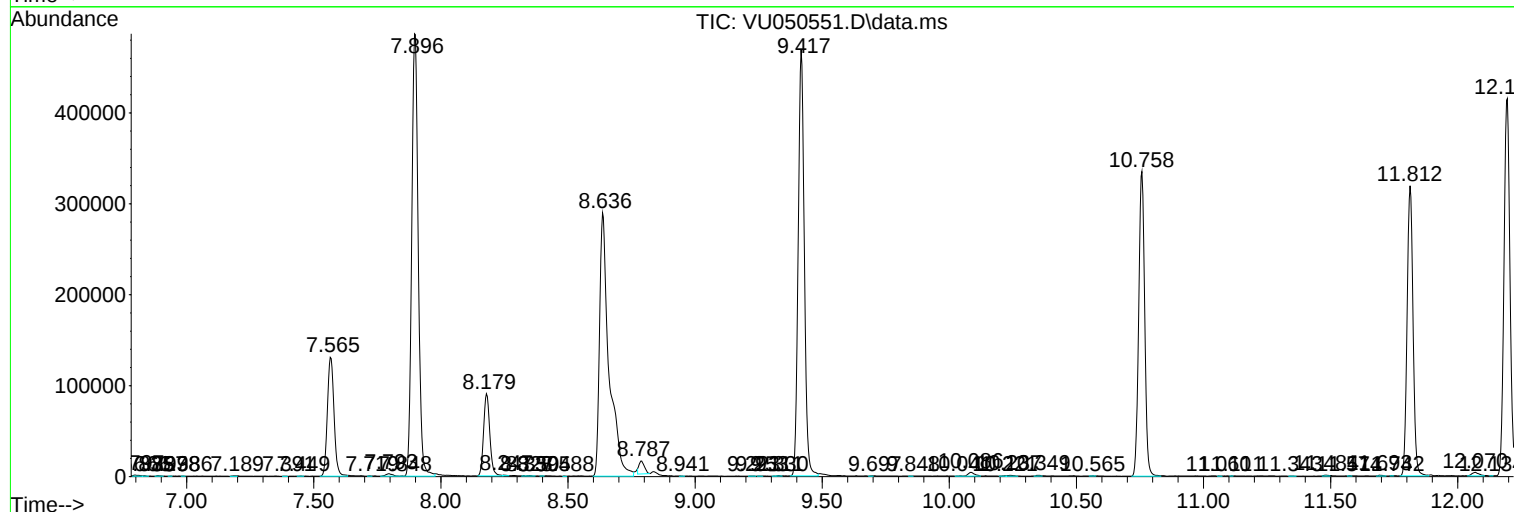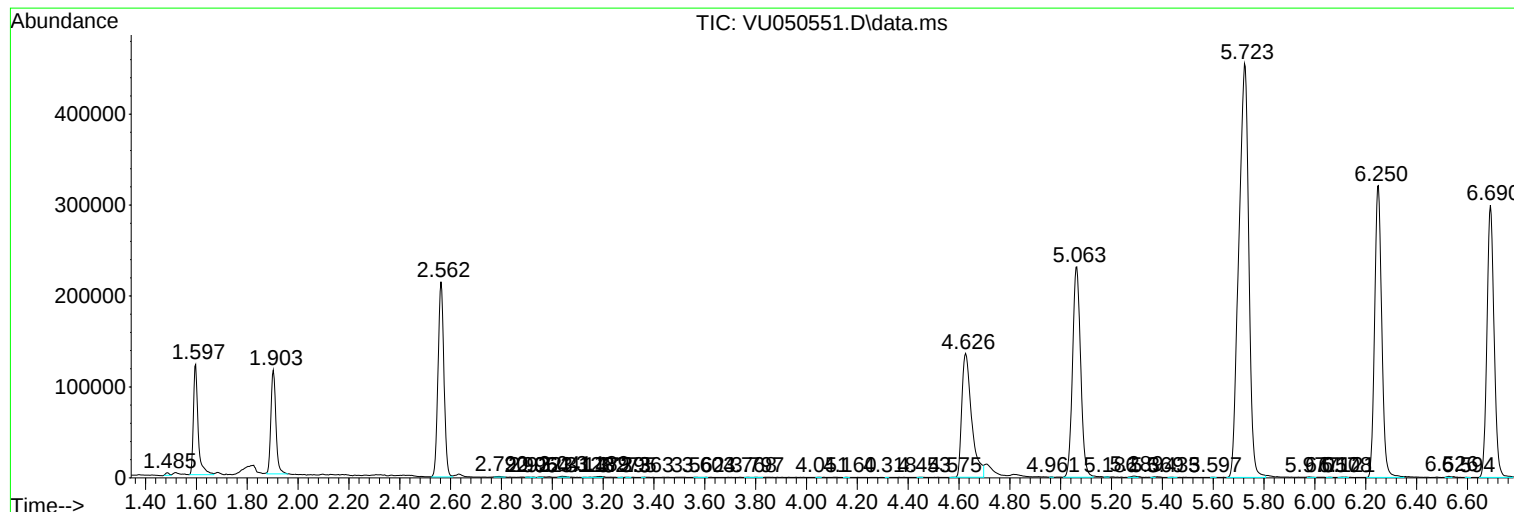

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050551.D
Acq On : 31 Aug 2022 16:09
Operator : SY/MD
Sample : N4440-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050551.D
Acq On : 31 Aug 2022 16:09
Operator : SY/MD
Sample : N4440-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc