

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050552.D
 Acq On : 31 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	3190	3387	0.27%	0.041%
2	1.517	51	55	59	rBV2	2299	2526	0.20%	0.030%
3	1.597	72	80	99	rBV	118438	152118	12.26%	1.831%
4	1.903	167	175	192	rVB	115541	157062	12.66%	1.891%
5	2.562	368	380	395	rBV	212293	342205	27.59%	4.120%
6	2.636	395	403	417	rVB	5694	11071	0.89%	0.133%
7	2.790	442	451	453	rBV4	917	1041	0.08%	0.013%
8	2.816	457	459	463	rVB2	497	309	0.02%	0.004%
9	2.880	475	479	483	rBV2	251	260	0.02%	0.003%
10	2.916	483	490	494	rBV4	417	564	0.05%	0.007%
11	2.957	500	503	511	rVB3	511	707	0.06%	0.009%
12	3.041	521	529	537	rBV4	1001	1569	0.13%	0.019%
13	3.121	550	554	561	rBV	760	744	0.06%	0.009%
14	3.170	564	569	571	rBV	702	664	0.05%	0.008%
15	3.189	572	575	584	rVB3	840	945	0.08%	0.011%
16	3.658	718	721	727	rVB	298	301	0.02%	0.004%
17	3.694	727	732	740	rBV	285	477	0.04%	0.006%
18	3.909	797	799	804	rVV2	260	210	0.02%	0.003%
19	3.935	804	807	813	rVB2	188	209	0.02%	0.003%
20	4.009	821	830	838	rBV2	443	795	0.06%	0.010%
21	4.080	848	852	856	rBV2	252	205	0.02%	0.002%
22	4.105	857	860	865	rVB2	301	241	0.02%	0.003%
23	4.189	883	886	890	rVB	285	213	0.02%	0.003%
24	4.571	1001	1005	1009	rVB2	334	246	0.02%	0.003%
25	4.629	1009	1023	1066	rBV	131304	386457	31.16%	4.653%
26	5.060	1136	1157	1181	rBV	220794	491318	39.61%	5.915%
27	5.208	1200	1203	1206	rBV2	360	242	0.02%	0.003%
28	5.288	1221	1228	1239	rVB5	1394	2571	0.21%	0.031%
29	5.366	1249	1252	1255	rBV2	504	462	0.04%	0.006%
30	5.723	1342	1363	1395	rBV2	455024	1240295	100.00%	14.932%
31	5.890	1411	1415	1418	rBV2	499	371	0.03%	0.004%
32	5.983	1438	1444	1448	rVB5	611	720	0.06%	0.009%
33	6.028	1453	1458	1461	rBV3	304	307	0.02%	0.004%
34	6.096	1473	1479	1480	rBV	224	211	0.02%	0.003%
35	6.128	1486	1489	1497	rVB3	435	357	0.03%	0.004%
36	6.250	1512	1527	1557	rBV	337919	644811	51.99%	7.763%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050552.D
 Acq On : 31 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.510	1602	1608	1609	rBV2	330	313	0.03%	0.004%
38	6.526	1609	1613	1614	rBV2	704	519	0.04%	0.006%
39	6.597	1632	1635	1640	rVB3	519	351	0.03%	0.004%
40	6.690	1647	1664	1686	rBV	294934	579166	46.70%	6.973%
41	6.796	1695	1697	1700	rBV4	595	348	0.03%	0.004%
42	6.993	1755	1758	1763	rVB2	234	218	0.02%	0.003%
43	7.179	1810	1816	1817	rBV3	788	606	0.05%	0.007%
44	7.192	1817	1820	1825	rVB3	800	693	0.06%	0.008%
45	7.259	1834	1841	1844	rBV2	263	327	0.03%	0.004%
46	7.565	1923	1936	1964	rVV	131377	235958	19.02%	2.841%
47	7.899	2026	2040	2063	rBV	483863	853560	68.82%	10.276%
48	8.179	2116	2127	2143	rBV	89190	152972	12.33%	1.842%
49	8.436	2204	2207	2209	rBV	358	235	0.02%	0.003%
50	8.555	2239	2244	2249	rVB3	462	486	0.04%	0.006%
51	8.639	2257	2270	2304	rBV5	276143	742119	59.83%	8.934%
52	8.874	2340	2343	2346	rBV3	450	249	0.02%	0.003%
53	9.417	2499	2512	2536	rBV	474963	795677	64.15%	9.579%
54	9.967	2680	2683	2689	rVB2	419	349	0.03%	0.004%
55	10.002	2689	2694	2697	rBV2	301	352	0.03%	0.004%
56	10.047	2706	2708	2713	rVV2	307	232	0.02%	0.003%
57	10.079	2715	2718	2722	rVV2	217	215	0.02%	0.003%
58	10.105	2722	2726	2729	rVB2	414	389	0.03%	0.005%
59	10.484	2837	2844	2849	rBV2	444	565	0.05%	0.007%
60	10.684	2903	2906	2911	rVB	310	254	0.02%	0.003%
61	10.758	2916	2929	2949	rBV	410162	655409	52.84%	7.891%
62	10.880	2964	2967	2974	rVB2	230	209	0.02%	0.003%
63	10.915	2974	2978	2982	rBV2	395	352	0.03%	0.004%
64	10.999	3000	3004	3007	rBV	248	249	0.02%	0.003%
65	11.304	3098	3099	3109	rVB2	524	648	0.05%	0.008%
66	11.494	3155	3158	3163	rVB2	308	251	0.02%	0.003%
67	11.526	3163	3168	3174	rBV2	189	275	0.02%	0.003%
68	11.571	3176	3182	3187	rBV	244	210	0.02%	0.003%
69	11.812	3244	3257	3278	rBV	235915	377014	30.40%	4.539%
70	11.973	3303	3307	3313	rVB2	308	330	0.03%	0.004%
71	12.005	3313	3317	3323	rBV2	233	309	0.02%	0.004%
72	12.070	3326	3337	3346	rBV6	2457	4209	0.34%	0.051%
73	12.111	3346	3350	3352	rBV	282	202	0.02%	0.002%
74	12.192	3362	3375	3391	rBV	269293	446222	35.98%	5.372%
75	12.317	3410	3414	3417	rVB3	513	278	0.02%	0.003%
76	12.436	3447	3451	3454	rBV2	266	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050552.D
 Acq On : 31 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	12.520	3474	3477	3482	rVB2	260	211	0.02%	0.003%
78	12.542	3482	3484	3487	rBV	354	247	0.02%	0.003%
79	12.793	3558	3562	3567	rVB2	278	325	0.03%	0.004%
80	12.819	3567	3570	3571	rBV2	341	208	0.02%	0.003%
81	13.005	3620	3628	3630	rBV2	362	455	0.04%	0.005%
82	13.089	3650	3654	3658	rBV	447	362	0.03%	0.004%
83	13.176	3676	3681	3682	rBV	281	269	0.02%	0.003%
84	13.201	3684	3689	3693	rVV3	274	304	0.02%	0.004%
85	13.369	3739	3741	3745	rVB2	376	228	0.02%	0.003%
86	13.494	3776	3780	3785	rVB2	423	353	0.03%	0.004%
87	13.542	3792	3795	3799	rVB3	416	401	0.03%	0.005%
88	13.574	3799	3805	3806	rBV2	297	265	0.02%	0.003%
89	13.613	3814	3817	3820	rBV	288	253	0.02%	0.003%
90	13.774	3863	3867	3870	rBV	318	315	0.03%	0.004%
91	13.841	3884	3888	3890	rBV2	343	319	0.03%	0.004%
92	13.999	3935	3937	3941	rBV	352	262	0.02%	0.003%
93	14.143	3980	3982	3986	rBV3	308	254	0.02%	0.003%
94	14.423	4065	4069	4072	rBV2	285	240	0.02%	0.003%
95	15.021	4252	4255	4260	rBV2	366	396	0.03%	0.005%
96	15.082	4271	4274	4279	rVB3	411	381	0.03%	0.005%
97	15.131	4285	4289	4291	rBV2	331	252	0.02%	0.003%
98	15.420	4376	4379	4383	rBV3	498	419	0.03%	0.005%
99	15.684	4459	4461	4465	rVB2	525	341	0.03%	0.004%
100	15.848	4509	4512	4516	rBV2	712	500	0.04%	0.006%




Sum of corrected areas: 8306276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050552.D
Acq On : 31 Aug 2022 16:32
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

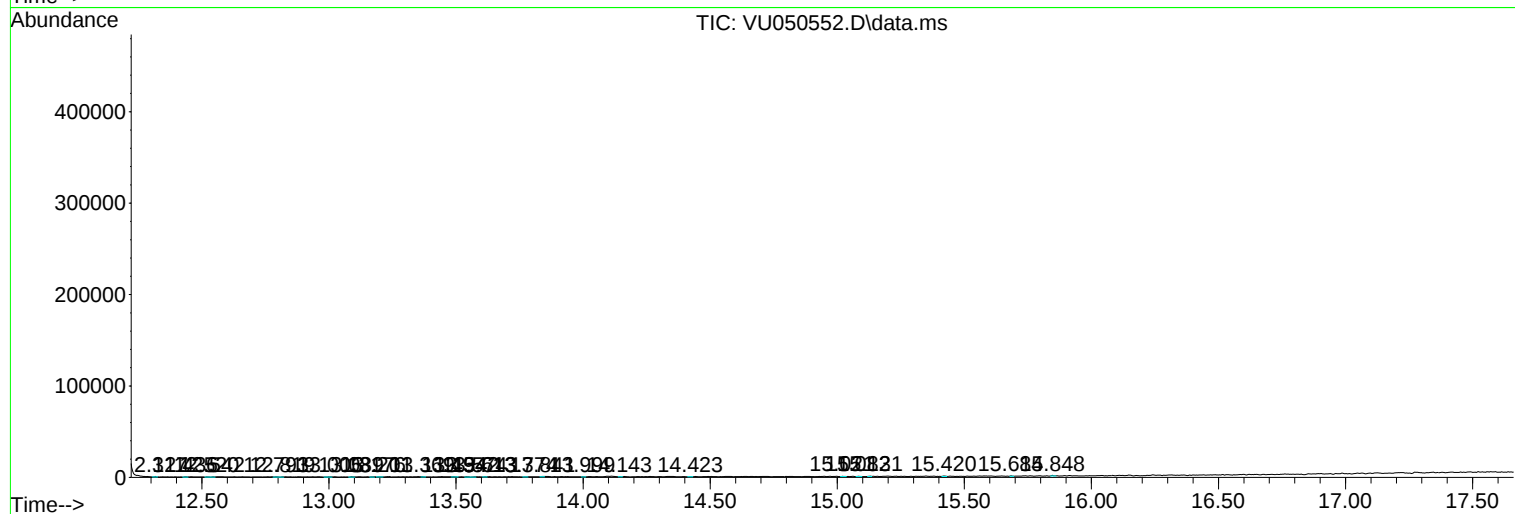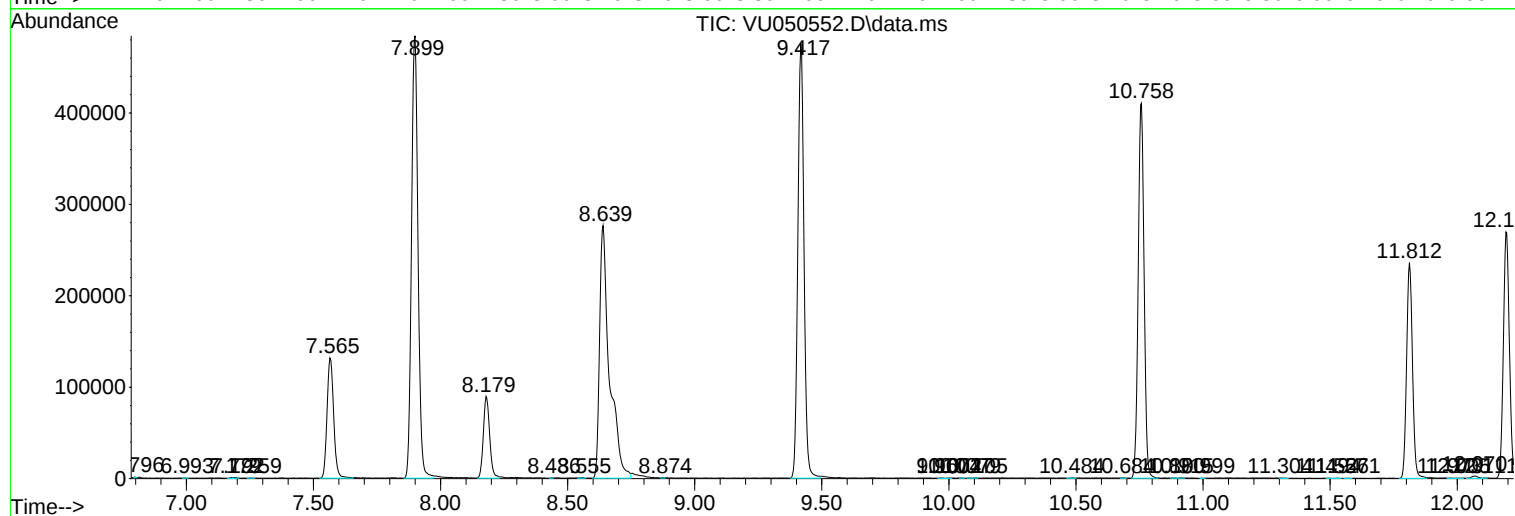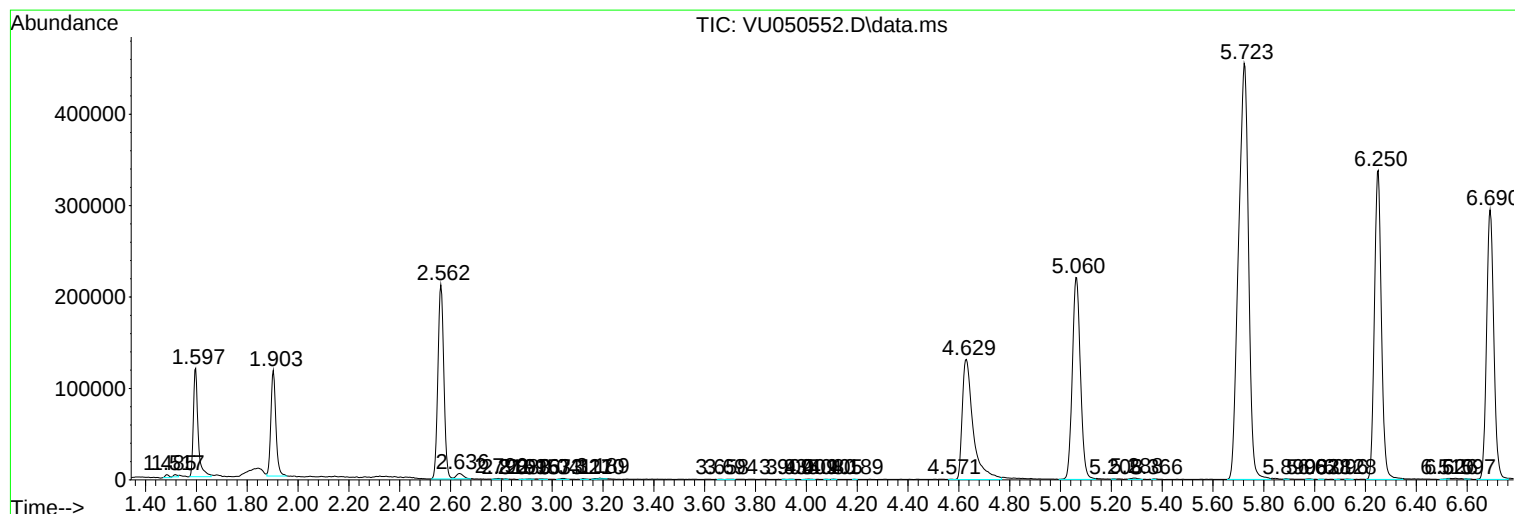

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050552.D
Acq On : 31 Aug 2022 16:32
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050552.D
Acq On : 31 Aug 2022 16:32
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc