

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050559.D
 Acq On : 31 Aug 2022 19:18
 Operator : SY/MD
 Sample : N4345-20ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	88	rBV	68908	95488	6.72%	0.920%
2	2.533	358	371	393	rBV	259792	424087	29.84%	4.084%
3	2.742	433	436	438	rVB2	240	124	0.01%	0.001%
4	2.755	438	440	442	rBV	348	165	0.01%	0.002%
5	2.874	474	477	481	rVB2	253	245	0.02%	0.002%
6	2.899	481	485	487	rBV	187	169	0.01%	0.002%
7	2.977	506	509	513	rBV	301	190	0.01%	0.002%
8	3.028	517	525	540	rVV4	4315	8363	0.59%	0.081%
9	3.182	556	573	596	rBV2	6437	18332	1.29%	0.177%
10	3.362	627	629	631	rBV2	303	200	0.01%	0.002%
11	3.427	645	649	651	rBV	195	160	0.01%	0.002%
12	3.639	712	715	717	rVB	245	144	0.01%	0.001%
13	3.674	721	726	728	rBV3	351	333	0.02%	0.003%
14	3.774	754	757	759	rBV	269	210	0.01%	0.002%
15	3.816	767	770	773	rBV2	169	137	0.01%	0.001%
16	3.903	795	797	803	rVB2	219	172	0.01%	0.002%
17	3.957	811	814	817	rBV2	170	143	0.01%	0.001%
18	4.009	828	830	834	rBV	177	98	0.01%	0.001%
19	4.038	834	839	843	rVB2	224	262	0.02%	0.003%
20	4.169	877	880	882	rVB2	181	107	0.01%	0.001%
21	4.182	882	884	886	rBV	200	126	0.01%	0.001%
22	4.301	918	921	922	rBV	208	118	0.01%	0.001%
23	4.423	955	959	961	rBV	206	122	0.01%	0.001%
24	4.446	962	966	970	rVB	324	300	0.02%	0.003%
25	4.472	970	974	976	rBV	248	191	0.01%	0.002%
26	4.587	1008	1010	1013	rVB2	213	123	0.01%	0.001%
27	4.645	1013	1028	1072	rBV	95025	345137	24.28%	3.324%
28	5.060	1140	1157	1185	rBV	239508	554700	39.02%	5.342%
29	5.211	1202	1204	1211	rVB3	502	494	0.03%	0.005%
30	5.279	1219	1225	1226	rBV2	528	538	0.04%	0.005%
31	5.333	1240	1242	1246	rBV	187	105	0.01%	0.001%
32	5.356	1246	1249	1250	rBV2	235	159	0.01%	0.002%
33	5.513	1296	1298	1302	rVB2	166	121	0.01%	0.001%
34	5.716	1342	1361	1395	rBV2	555424	1421409	100.00%	13.689%
35	5.912	1418	1422	1424	rBV	232	210	0.01%	0.002%
36	5.976	1433	1442	1464	rBV7	5945	16546	1.16%	0.159%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050559.D
 Acq On : 31 Aug 2022 19:18
 Operator : SY/MD
 Sample : N4345-20ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.247	1506	1526	1555	rBV	477174	956568	67.30%	9.212%
38	6.468	1592	1595	1597	rBV2	186	107	0.01%	0.001%
39	6.523	1602	1612	1622	rBV7	3022	5837	0.41%	0.056%
40	6.610	1625	1639	1648	rBV4	3516	7299	0.51%	0.070%
41	6.690	1649	1664	1692	rVB	316766	643326	45.26%	6.196%
42	6.806	1693	1700	1705	rVV5	705	772	0.05%	0.007%
43	6.896	1724	1728	1732	rBV	88	107	0.01%	0.001%
44	6.992	1754	1758	1764	rBV	261	280	0.02%	0.003%
45	7.066	1779	1781	1784	rVB	186	122	0.01%	0.001%
46	7.092	1784	1789	1790	rBV	167	128	0.01%	0.001%
47	7.105	1790	1793	1796	rVB2	170	105	0.01%	0.001%
48	7.121	1796	1798	1803	rVB	172	112	0.01%	0.001%
49	7.227	1812	1831	1843	rBV7	2632	6826	0.48%	0.066%
50	7.311	1853	1857	1861	rBV2	459	429	0.03%	0.004%
51	7.359	1870	1872	1879	rVB	259	156	0.01%	0.002%
52	7.401	1879	1885	1888	rBV	138	162	0.01%	0.002%
53	7.494	1911	1914	1916	rBV	247	176	0.01%	0.002%
54	7.565	1920	1936	1960	rBV	140547	274765	19.33%	2.646%
55	7.896	2025	2039	2062	rBV	613433	1109515	78.06%	10.685%
56	8.102	2101	2103	2108	rBV2	191	158	0.01%	0.002%
57	8.182	2116	2128	2146	rBV2	92871	179484	12.63%	1.729%
58	8.279	2156	2158	2160	rBV	344	132	0.01%	0.001%
59	8.298	2163	2164	2169	rVB	373	207	0.01%	0.002%
60	8.362	2182	2184	2189	rVB	511	319	0.02%	0.003%
61	8.504	2223	2228	2234	rBV2	333	306	0.02%	0.003%
62	8.549	2234	2242	2256	rBV3	9429	15569	1.10%	0.150%
63	8.661	2258	2277	2310	rBV2	275302	731085	51.43%	7.041%
64	8.870	2339	2342	2347	rBV2	462	416	0.03%	0.004%
65	8.928	2358	2360	2364	rBV	270	228	0.02%	0.002%
66	9.063	2400	2402	2407	rBV2	230	172	0.01%	0.002%
67	9.124	2416	2421	2423	rBV	211	207	0.01%	0.002%
68	9.240	2454	2457	2459	rVB	242	149	0.01%	0.001%
69	9.420	2499	2513	2532	rBV	604383	1119323	78.75%	10.780%
70	9.635	2577	2580	2583	rBV2	138	119	0.01%	0.001%
71	9.706	2594	2602	2605	rBV2	220	321	0.02%	0.003%
72	9.761	2616	2619	2625	rBV2	222	203	0.01%	0.002%
73	10.015	2696	2698	2702	rVB	208	108	0.01%	0.001%
74	10.037	2702	2705	2708	rBV	281	172	0.01%	0.002%
75	10.086	2717	2720	2721	rBV	192	114	0.01%	0.001%
76	10.198	2751	2755	2756	rBV	240	115	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050559.D
 Acq On : 31 Aug 2022 19:18
 Operator : SY/MD
 Sample : N4345-20ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.372	2807	2809	2815	rVB	218	143	0.01%	0.001%
78	10.410	2815	2821	2825	rBV2	277	321	0.02%	0.003%
79	10.504	2847	2850	2855	rBV2	171	146	0.01%	0.001%
80	10.574	2868	2872	2873	rBV	199	121	0.01%	0.001%
81	10.635	2886	2891	2896	rBV2	461	691	0.05%	0.007%
82	10.764	2917	2931	2950	rBV	438608	726996	51.15%	7.001%
83	10.986	2996	3000	3003	rBV	257	243	0.02%	0.002%
84	11.050	3017	3020	3023	rBV2	191	138	0.01%	0.001%
85	11.118	3036	3041	3047	rVB4	684	910	0.06%	0.009%
86	11.169	3055	3057	3059	rBV2	212	140	0.01%	0.001%
87	11.446	3141	3143	3146	rVB2	267	152	0.01%	0.001%
88	11.539	3167	3172	3174	rBV2	296	295	0.02%	0.003%
89	11.574	3180	3183	3185	rBV	189	155	0.01%	0.001%
90	11.693	3216	3220	3227	rBV	325	348	0.02%	0.003%
91	11.761	3239	3241	3244	rBV	193	99	0.01%	0.001%
92	11.815	3245	3258	3278	rBV	546145	858566	60.40%	8.268%
93	11.983	3308	3310	3313	rVB2	264	132	0.01%	0.001%
94	12.195	3360	3376	3396	rBV	527480	847558	59.63%	8.162%
95	12.365	3425	3429	3431	rBV2	344	235	0.02%	0.002%
96	12.516	3474	3476	3482	rVB2	323	235	0.02%	0.002%
97	12.545	3482	3485	3486	rBV	339	186	0.01%	0.002%
98	12.745	3544	3547	3548	rBV2	213	130	0.01%	0.001%
99	13.661	3830	3832	3835	rBV2	353	229	0.02%	0.002%
100	14.024	3941	3945	3946	rBV	286	211	0.01%	0.002%




Sum of corrected areas: 10383607

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050559.D
Acq On : 31 Aug 2022 19:18
Operator : SY/MD
Sample : N4345-20ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

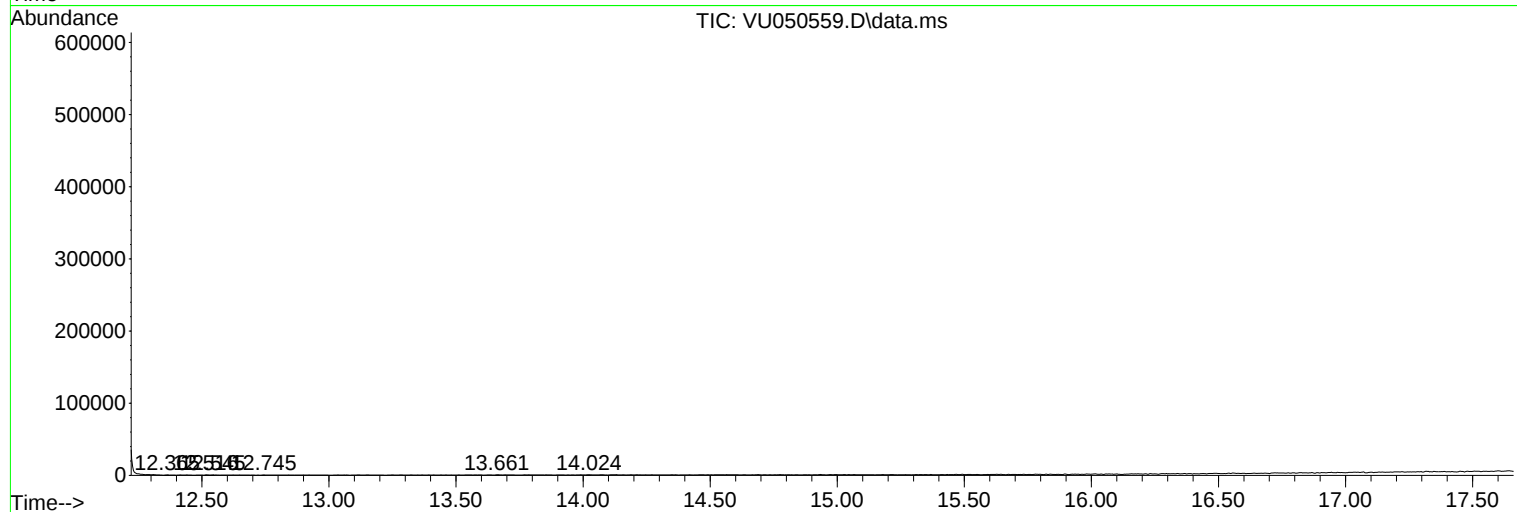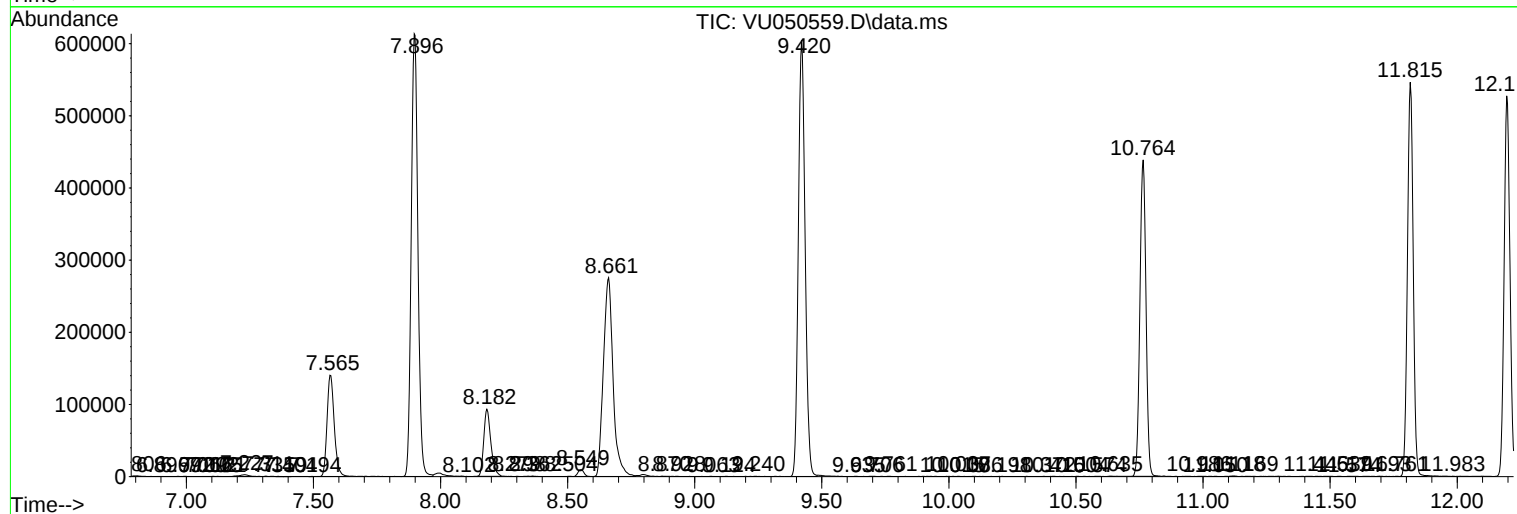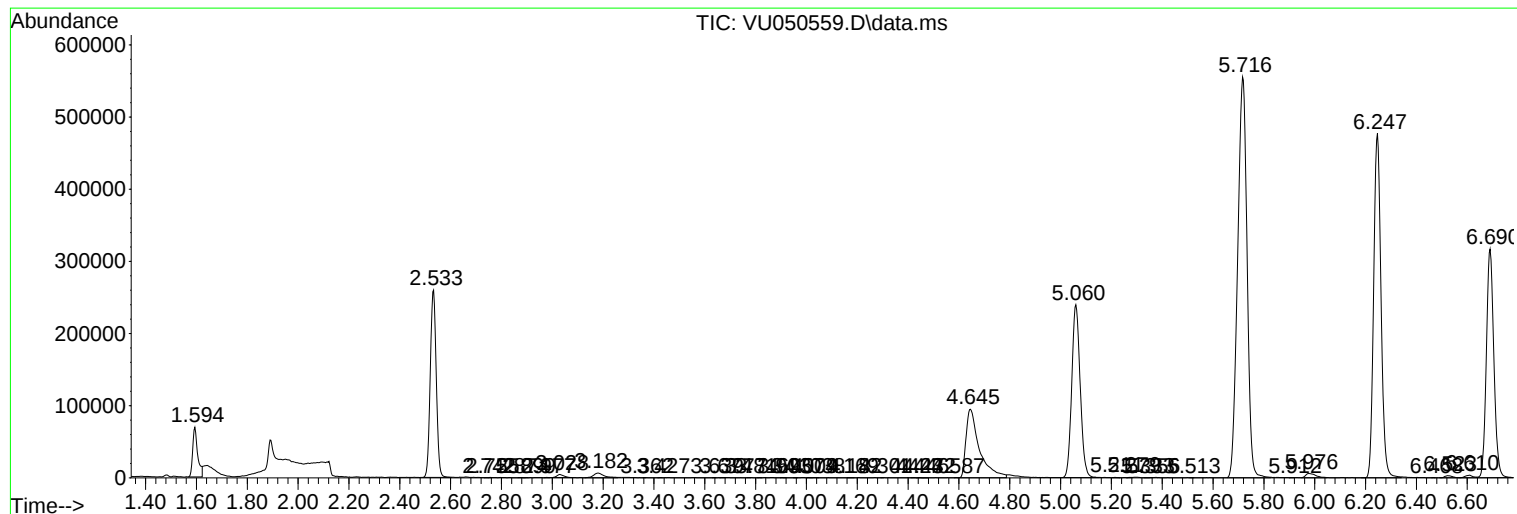

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050559.D
Acq On : 31 Aug 2022 19:18
Operator : SY/MD
Sample : N4345-20ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050559.D
Acq On : 31 Aug 2022 19:18
Operator : SY/MD
Sample : N4345-20ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------