

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050561.D
 Acq On : 31 Aug 2022 20:05
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	87	rBV	43667	58884	6.71%	0.914%
2	2.530	358	370	384	rBV	157601	256444	29.20%	3.981%
3	2.607	391	394	397	rVB2	309	202	0.02%	0.003%
4	2.623	397	399	400	rBV	328	157	0.02%	0.002%
5	2.752	436	439	443	rBV3	331	315	0.04%	0.005%
6	2.838	464	466	472	rVB	278	209	0.02%	0.003%
7	2.883	477	480	484	rBV2	186	131	0.01%	0.002%
8	2.906	484	487	492	rBV	195	181	0.02%	0.003%
9	2.935	492	496	497	rBV	228	136	0.02%	0.002%
10	3.028	516	525	541	rVB3	4520	9420	1.07%	0.146%
11	3.179	554	572	589	rBV	8130	22295	2.54%	0.346%
12	3.449	654	656	664	rVB2	294	250	0.03%	0.004%
13	3.674	722	726	728	rBV2	313	214	0.02%	0.003%
14	3.755	748	751	752	rBV2	245	120	0.01%	0.002%
15	3.842	775	778	781	rBV2	174	132	0.02%	0.002%
16	3.880	787	790	795	rVB2	193	127	0.01%	0.002%
17	3.964	812	816	820	rBV2	180	211	0.02%	0.003%
18	4.018	828	833	836	rBV2	215	213	0.02%	0.003%
19	4.054	841	844	846	rBV	196	124	0.01%	0.002%
20	4.330	928	930	933	rVV	223	141	0.02%	0.002%
21	4.388	945	948	951	rBV2	229	142	0.02%	0.002%
22	4.578	1001	1007	1011	rBV2	180	197	0.02%	0.003%
23	4.649	1016	1029	1078	rBV	58113	213465	24.31%	3.314%
24	4.989	1132	1135	1138	rBV	280	175	0.02%	0.003%
25	5.060	1140	1157	1182	rVV2	147036	342271	38.98%	5.313%
26	5.288	1222	1228	1231	rBV4	704	968	0.11%	0.015%
27	5.362	1248	1251	1253	rBV2	280	169	0.02%	0.003%
28	5.549	1304	1309	1312	rVB	278	185	0.02%	0.003%
29	5.716	1341	1361	1385	rBV2	345900	878177	100.00%	13.632%
30	5.980	1429	1443	1460	rBV4	6101	15512	1.77%	0.241%
31	6.124	1484	1488	1491	rVB2	174	131	0.01%	0.002%
32	6.157	1496	1498	1501	rVB2	259	152	0.02%	0.002%
33	6.247	1511	1526	1553	rBV	288023	579699	66.01%	8.999%
34	6.533	1606	1615	1622	rBV6	2684	4599	0.52%	0.071%
35	6.604	1628	1637	1650	rBV5	2960	6180	0.70%	0.096%
36	6.690	1650	1664	1686	rVV	191676	394317	44.90%	6.121%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050561.D
 Acq On : 31 Aug 2022 20:05
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.800	1695	1698	1703	rVB2	394	337	0.04%	0.005%
38	6.829	1703	1707	1710	rVB2	241	149	0.02%	0.002%
39	6.848	1710	1713	1716	rBV2	198	174	0.02%	0.003%
40	6.980	1751	1754	1757	rBV3	328	218	0.02%	0.003%
41	7.031	1764	1770	1772	rBV	132	136	0.02%	0.002%
42	7.227	1815	1831	1841	rBV8	3226	6769	0.77%	0.105%
43	7.298	1851	1853	1855	rBV	267	157	0.02%	0.002%
44	7.440	1892	1897	1900	rBV2	332	353	0.04%	0.005%
45	7.565	1924	1936	1959	rBV	85189	164324	18.71%	2.551%
46	7.832	2015	2019	2022	rBV2	138	119	0.01%	0.002%
47	7.896	2025	2039	2059	rBV	375510	670813	76.39%	10.413%
48	8.128	2104	2111	2112	rBV2	221	194	0.02%	0.003%
49	8.182	2116	2128	2149	rVV2	54203	107119	12.20%	1.663%
50	8.288	2157	2161	2165	rBV2	237	268	0.03%	0.004%
51	8.327	2171	2173	2177	rBV2	230	148	0.02%	0.002%
52	8.446	2207	2210	2212	rBV	246	164	0.02%	0.003%
53	8.459	2212	2214	2217	rVB	251	119	0.01%	0.002%
54	8.478	2217	2220	2227	rVB2	356	280	0.03%	0.004%
55	8.552	2231	2243	2259	rVB	61224	101921	11.61%	1.582%
56	8.665	2259	2278	2308	rBV2	159597	440559	50.17%	6.839%
57	8.902	2349	2352	2354	rBV	190	147	0.02%	0.002%
58	8.922	2357	2358	2365	rVB2	281	188	0.02%	0.003%
59	8.986	2374	2378	2381	rBV	212	121	0.01%	0.002%
60	9.012	2381	2386	2390	rVV2	236	232	0.03%	0.004%
61	9.044	2394	2396	2399	rVB2	245	144	0.02%	0.002%
62	9.140	2423	2426	2430	rBB2	208	146	0.02%	0.002%
63	9.308	2472	2478	2481	rBV	246	281	0.03%	0.004%
64	9.420	2496	2513	2539	rBV	364745	688324	78.38%	10.685%
65	9.587	2562	2565	2568	rVB2	236	162	0.02%	0.003%
66	9.745	2608	2614	2620	rBV3	396	517	0.06%	0.008%
67	9.893	2656	2660	2664	rBV2	258	220	0.03%	0.003%
68	9.970	2681	2684	2686	rBV2	257	172	0.02%	0.003%
69	10.060	2709	2712	2716	rBV2	282	271	0.03%	0.004%
70	10.131	2731	2734	2738	rBV2	228	188	0.02%	0.003%
71	10.291	2780	2784	2786	rBV	226	175	0.02%	0.003%
72	10.308	2786	2789	2794	rVV	215	190	0.02%	0.003%
73	10.333	2794	2797	2800	rBV	214	161	0.02%	0.002%
74	10.410	2818	2821	2826	rVB2	178	162	0.02%	0.003%
75	10.491	2843	2846	2849	rBV	207	124	0.01%	0.002%
76	10.600	2877	2880	2882	rVB2	278	181	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050561.D
 Acq On : 31 Aug 2022 20:05
 Operator : SY/MD
 Sample : N4363-11ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVW6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.706	2911	2913	2917	rBV	203	159	0.02%	0.002%
78	10.764	2917	2931	2946	rBV	267096	448421	51.06%	6.961%
79	10.983	2994	2999	3002	rBV2	392	291	0.03%	0.005%
80	11.195	3062	3065	3067	rBV2	167	132	0.02%	0.002%
81	11.298	3093	3097	3099	rBV	241	179	0.02%	0.003%
82	11.359	3112	3116	3120	rBV2	277	235	0.03%	0.004%
83	11.616	3192	3196	3199	rBV	191	192	0.02%	0.003%
84	11.774	3240	3245	3246	rBV2	211	176	0.02%	0.003%
85	11.816	3246	3258	3282	rVV	323931	511856	58.29%	7.946%
86	12.025	3321	3323	3327	rVB2	295	172	0.02%	0.003%
87	12.050	3327	3331	3336	rBV2	348	394	0.04%	0.006%
88	12.195	3363	3376	3396	rBV	311168	504474	57.45%	7.831%
89	12.758	3549	3551	3554	rBV	328	184	0.02%	0.003%
90	12.838	3574	3576	3582	rVB	336	233	0.03%	0.004%
91	12.896	3592	3594	3595	rBV	307	126	0.01%	0.002%
92	12.944	3606	3609	3612	rBV3	342	279	0.03%	0.004%
93	13.050	3640	3642	3646	rBV2	264	148	0.02%	0.002%
94	13.089	3652	3654	3656	rBV	212	124	0.01%	0.002%
95	13.237	3698	3700	3703	rBV	228	153	0.02%	0.002%
96	13.365	3734	3740	3742	rBV2	377	443	0.05%	0.007%
97	13.459	3765	3769	3772	rBV2	397	344	0.04%	0.005%
98	13.491	3775	3779	3781	rBV2	329	246	0.03%	0.004%
99	13.613	3815	3817	3821	rVB2	337	163	0.02%	0.003%
100	13.812	3876	3879	3880	rBV2	543	227	0.03%	0.004%




Sum of corrected areas: 6442023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050561.D
Acq On : 31 Aug 2022 20:05
Operator : SY/MD
Sample : N4363-11ME
Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVW6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

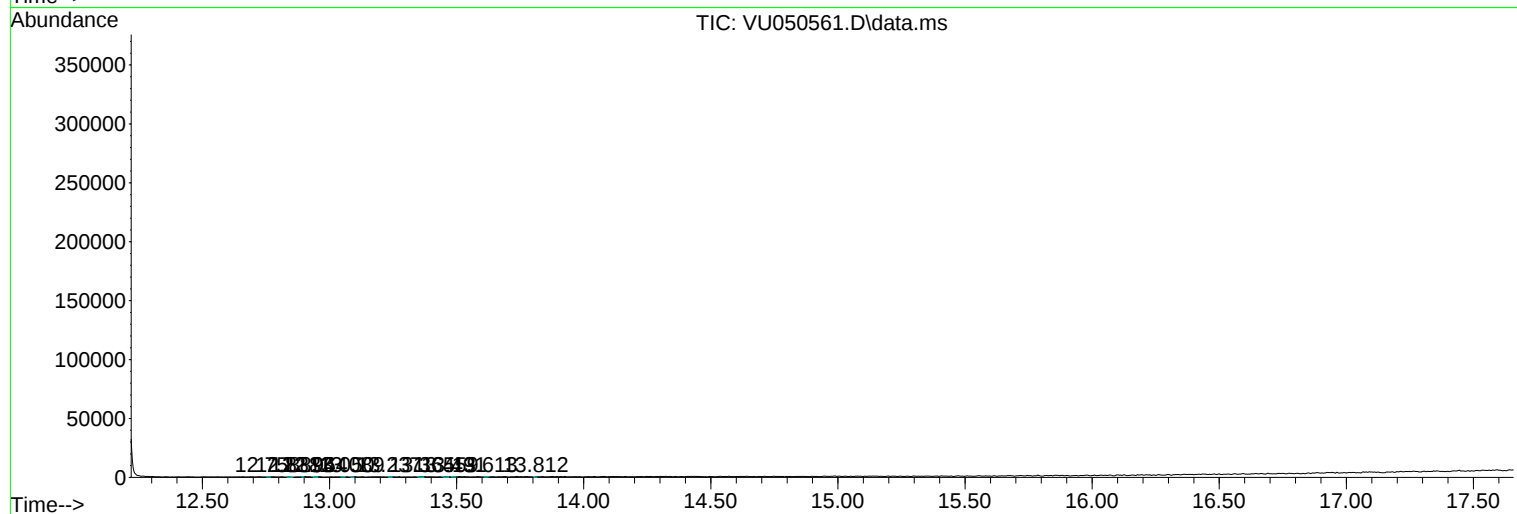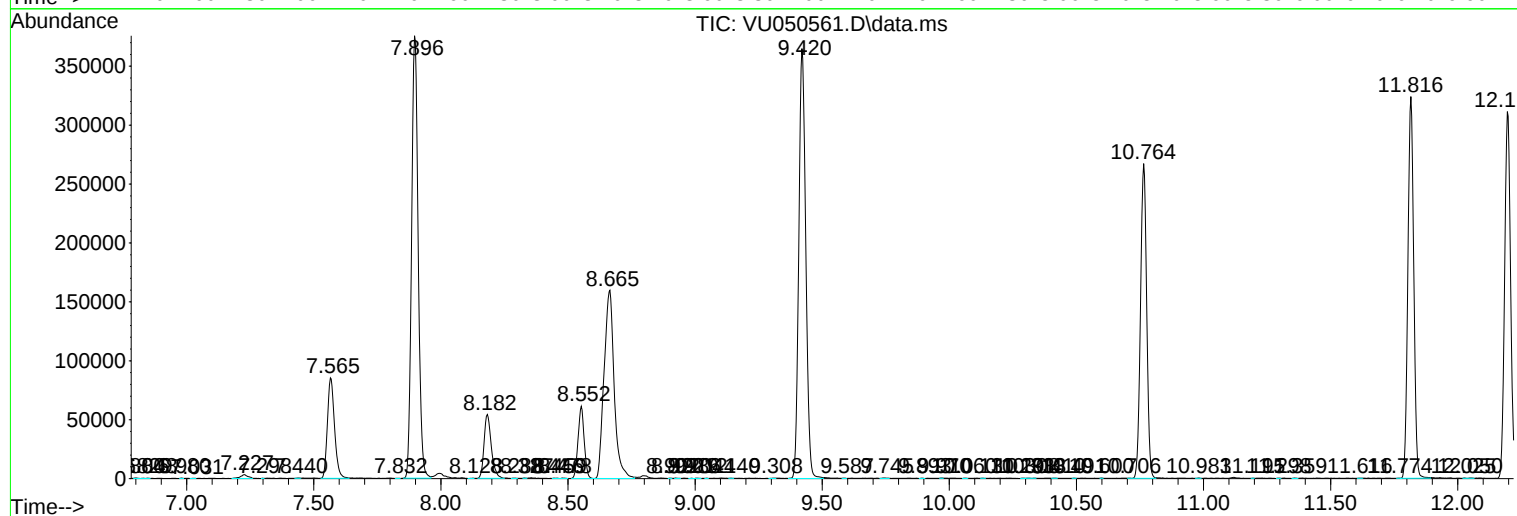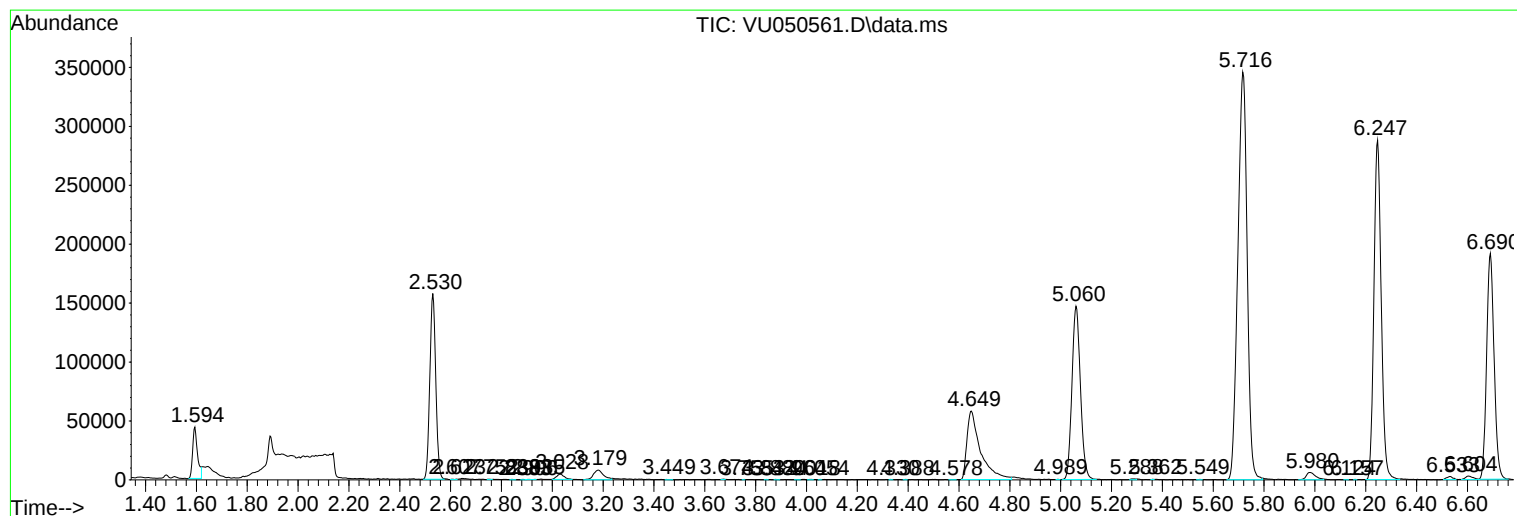

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050561.D
Acq On : 31 Aug 2022 20:05
Operator : SY/MD
Sample : N4363-11ME
Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVW6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050561.D
Acq On : 31 Aug 2022 20:05
Operator : SY/MD
Sample : N4363-11ME
Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVW6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc