

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050562.D
 Acq On : 31 Aug 2022 20:29
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	40	44	49	rVB3	2530	2262	0.14%	0.019%
2	1.594	71	79	104	rBV	102894	173027	10.41%	1.436%
3	1.780	130	137	138	rBV3	2250	1963	0.12%	0.016%
4	1.887	164	170	194	rBV	82877	139133	8.37%	1.155%
5	2.215	269	272	276	rBV3	435	424	0.03%	0.004%
6	2.327	304	307	310	rVB2	270	194	0.01%	0.002%
7	2.456	344	347	350	rBV	306	224	0.01%	0.002%
8	2.549	363	376	394	rVB	303506	488548	29.39%	4.055%
9	2.639	400	404	408	rBV3	488	555	0.03%	0.005%
10	2.771	442	445	450	rVV2	245	234	0.01%	0.002%
11	2.957	500	503	505	rBV2	349	205	0.01%	0.002%
12	3.034	519	527	539	rVB3	3686	6629	0.40%	0.055%
13	3.182	557	573	587	rBV2	4086	11104	0.67%	0.092%
14	3.443	651	654	658	rBV2	240	201	0.01%	0.002%
15	3.822	767	772	777	rBV2	264	286	0.02%	0.002%
16	4.073	847	850	857	rVB	293	239	0.01%	0.002%
17	4.189	881	886	892	rBV2	262	313	0.02%	0.003%
18	4.285	913	916	919	rVB	366	292	0.02%	0.002%
19	4.314	920	925	927	rBV2	356	341	0.02%	0.003%
20	4.465	968	972	977	rBV	281	350	0.02%	0.003%
21	4.510	983	986	988	rBV	269	198	0.01%	0.002%
22	4.632	1011	1024	1078	rVV2	127280	413760	24.89%	3.434%
23	5.060	1140	1157	1178	rBV	292722	648769	39.02%	5.384%
24	5.202	1198	1201	1205	rVV4	567	460	0.03%	0.004%
25	5.282	1221	1226	1230	rBV4	657	904	0.05%	0.008%
26	5.378	1253	1256	1258	rBV2	326	264	0.02%	0.002%
27	5.719	1341	1362	1387	rBV2	635464	1662513	100.00%	13.798%
28	5.867	1405	1408	1411	rBV	312	226	0.01%	0.002%
29	5.976	1433	1442	1459	rVB8	2783	6305	0.38%	0.052%
30	6.041	1459	1462	1466	rBV3	327	323	0.02%	0.003%
31	6.102	1478	1481	1484	rBV2	279	229	0.01%	0.002%
32	6.247	1511	1526	1556	rBV	501138	938850	56.47%	7.792%
33	6.375	1564	1566	1570	rVB	435	280	0.02%	0.002%
34	6.529	1606	1614	1625	rVB9	2531	4004	0.24%	0.033%
35	6.597	1629	1635	1646	rVB4	1291	2302	0.14%	0.019%
36	6.690	1646	1664	1684	rBV	380287	751954	45.23%	6.241%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050562.D
 Acq On : 31 Aug 2022 20:29
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.800	1696	1698	1699	rBV	575	279	0.02%	0.002%
38	7.195	1814	1821	1822	rBV2	874	962	0.06%	0.008%
39	7.269	1842	1844	1848	rVB2	258	189	0.01%	0.002%
40	7.565	1923	1936	1958	rBV	174462	314574	18.92%	2.611%
41	7.700	1975	1978	1980	rBV2	296	197	0.01%	0.002%
42	7.896	2024	2039	2061	rBV	740106	1287932	77.47%	10.689%
43	8.124	2107	2110	2113	rBV2	308	199	0.01%	0.002%
44	8.179	2116	2127	2146	rBV	118722	210874	12.68%	1.750%
45	8.407	2196	2198	2205	rVB	240	202	0.01%	0.002%
46	8.459	2210	2214	2217	rBV	356	232	0.01%	0.002%
47	8.504	2225	2228	2233	rBV2	258	221	0.01%	0.002%
48	8.552	2233	2243	2253	rBV2	24036	39827	2.40%	0.331%
49	8.645	2257	2272	2301	rBV2	432548	933493	56.15%	7.747%
50	8.854	2336	2337	2340	rVB	420	188	0.01%	0.002%
51	8.873	2340	2343	2348	rVB3	363	291	0.02%	0.002%
52	8.928	2358	2360	2363	rVB	369	212	0.01%	0.002%
53	8.951	2364	2367	2371	rVB	301	195	0.01%	0.002%
54	8.979	2373	2376	2379	rBV	394	203	0.01%	0.002%
55	9.041	2392	2395	2402	rVB	308	218	0.01%	0.002%
56	9.417	2499	2512	2538	rBV	664553	1121367	67.45%	9.307%
57	9.558	2553	2556	2559	rBV4	409	238	0.01%	0.002%
58	9.603	2566	2570	2575	rBV2	316	276	0.02%	0.002%
59	9.635	2575	2580	2585	rVB2	285	385	0.02%	0.003%
60	10.169	2743	2746	2749	rBV	258	199	0.01%	0.002%
61	10.455	2832	2835	2836	rBV2	390	230	0.01%	0.002%
62	10.761	2917	2930	2956	rBV	573905	924776	55.63%	7.675%
63	10.954	2987	2990	2994	rVB2	367	270	0.02%	0.002%
64	10.979	2994	2998	3001	rBV2	237	213	0.01%	0.002%
65	11.069	3020	3026	3029	rBV2	200	213	0.01%	0.002%
66	11.114	3036	3040	3046	rVB3	406	464	0.03%	0.004%
67	11.211	3065	3070	3073	rVB	236	194	0.01%	0.002%
68	11.246	3078	3081	3084	rVB2	266	190	0.01%	0.002%
69	11.301	3094	3098	3101	rBV2	234	218	0.01%	0.002%
70	11.420	3132	3135	3140	rVB2	270	258	0.02%	0.002%
71	11.558	3174	3178	3181	rBV2	321	316	0.02%	0.003%
72	11.812	3244	3257	3274	rBV	570675	889147	53.48%	7.379%
73	11.934	3292	3295	3299	rBV3	440	452	0.03%	0.004%
74	11.973	3305	3307	3312	rVB2	460	359	0.02%	0.003%
75	11.995	3312	3314	3317	rBV	277	232	0.01%	0.002%
76	12.040	3324	3328	3332	rBV2	395	312	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050562.D
 Acq On : 31 Aug 2022 20:29
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	12.195	3363	3376	3399	rBV	655172	1052825	63.33%	8.738%
78	12.359	3424	3427	3431	rBV2	613	566	0.03%	0.005%
79	12.407	3439	3442	3445	rVB	375	214	0.01%	0.002%
80	12.436	3445	3451	3454	rBV2	448	492	0.03%	0.004%
81	12.471	3459	3462	3464	rBV	341	210	0.01%	0.002%
82	12.896	3591	3594	3599	rBV2	245	200	0.01%	0.002%
83	13.015	3628	3631	3634	rBV2	246	199	0.01%	0.002%
84	13.240	3698	3701	3704	rVV2	266	201	0.01%	0.002%
85	13.327	3724	3728	3733	rVB2	486	483	0.03%	0.004%
86	13.491	3776	3779	3782	rBV	301	201	0.01%	0.002%
87	13.680	3835	3838	3840	rBV3	346	274	0.02%	0.002%
88	13.738	3848	3856	3860	rVB2	331	566	0.03%	0.005%
89	13.764	3860	3864	3868	rBV2	428	360	0.02%	0.003%
90	13.854	3888	3892	3896	rVB2	388	321	0.02%	0.003%
91	14.024	3942	3945	3948	rBV2	278	223	0.01%	0.002%
92	14.047	3949	3952	3958	rVV2	326	338	0.02%	0.003%
93	14.259	4014	4018	4021	rBV2	445	330	0.02%	0.003%
94	14.413	4063	4066	4069	rBV2	324	235	0.01%	0.002%
95	14.571	4112	4115	4117	rBV2	335	214	0.01%	0.002%
96	14.629	4126	4133	4142	rBV3	443	828	0.05%	0.007%
97	14.777	4177	4179	4182	rBV2	300	203	0.01%	0.002%
98	14.880	4208	4211	4213	rBV3	368	252	0.02%	0.002%
99	15.304	4341	4343	4349	rBV3	415	363	0.02%	0.003%
100	15.552	4417	4420	4423	rVB3	617	423	0.03%	0.004%


Sum of corrected areas: 12049183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050562.D
Acq On : 31 Aug 2022 20:29
Operator : SY/MD
Sample : N4345-13ME
Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

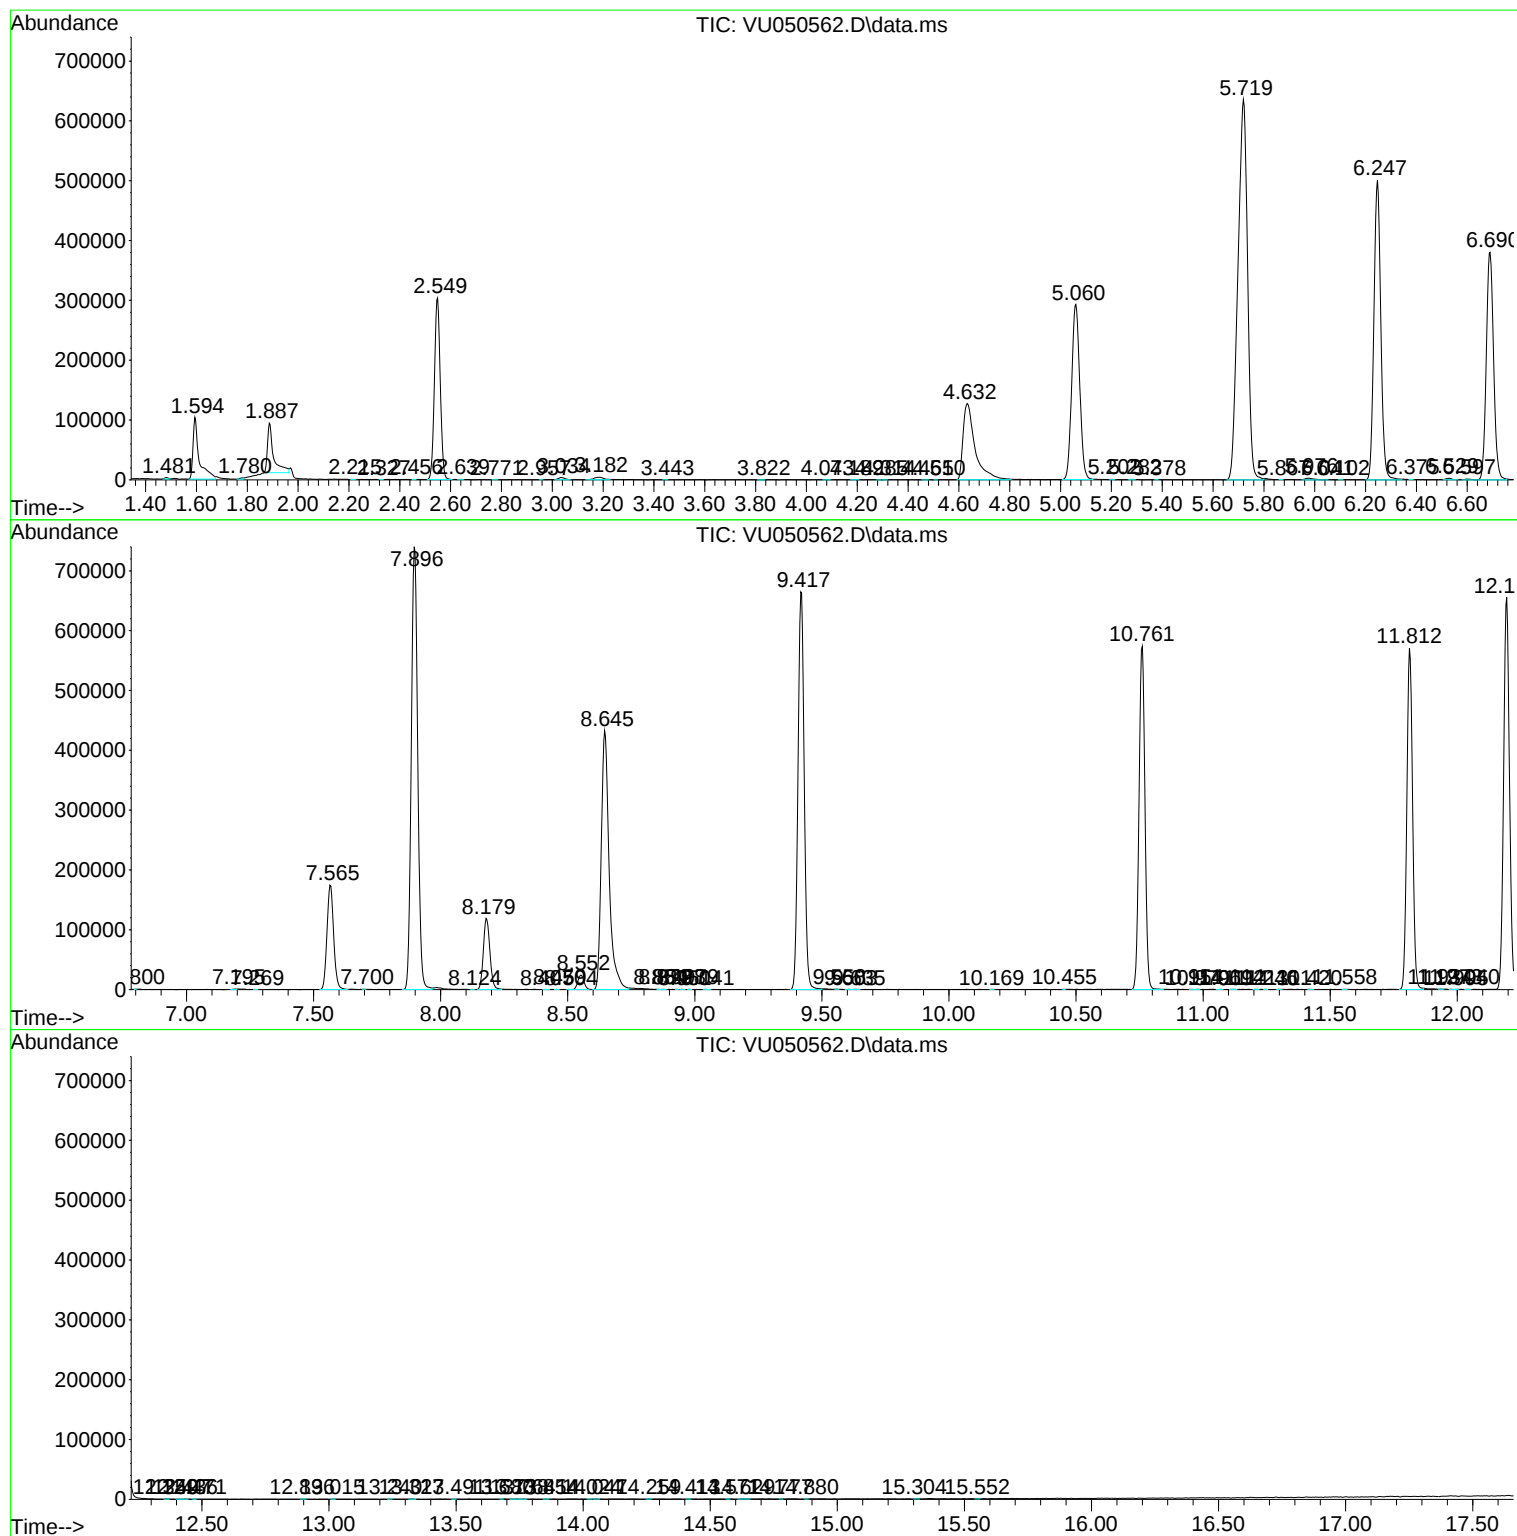

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050562.D
Acq On : 31 Aug 2022 20:29
Operator : SY/MD
Sample : N4345-13ME
Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050562.D
Acq On : 31 Aug 2022 20:29
Operator : SY/MD
Sample : N4345-13ME
Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc