

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050565.D
 Acq On : 31 Aug 2022 21:40
 Operator : SY/MD
 Sample : N4345-01MEDL 400X
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M

Title : VOC Analysis

Signal : TIC: VU050565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rBV	83285	102453	11.94%	1.443%
2	1.906	167	176	195	rVB	68931	92966	10.83%	1.309%
3	2.562	369	380	399	rVB	158408	255582	29.79%	3.599%
4	2.758	437	441	444	rBV2	187	154	0.02%	0.002%
5	2.777	444	447	450	rBV2	389	335	0.04%	0.005%
6	2.845	465	468	472	rBV2	197	160	0.02%	0.002%
7	2.906	482	487	489	rBV2	243	254	0.03%	0.004%
8	2.989	509	513	516	rBV2	247	234	0.03%	0.003%
9	3.047	522	531	539	rBV4	1322	2177	0.25%	0.031%
10	3.108	547	550	553	rVB2	190	143	0.02%	0.002%
11	3.137	553	559	562	rBV2	214	269	0.03%	0.004%
12	3.179	562	572	589	rVB2	3955	8961	1.04%	0.126%
13	3.285	602	605	608	rBV2	170	133	0.02%	0.002%
14	3.321	613	616	621	rBV2	209	204	0.02%	0.003%
15	3.346	621	624	628	rBV2	176	170	0.02%	0.002%
16	3.469	659	662	664	rBV	197	102	0.01%	0.001%
17	3.523	675	679	682	rVB2	168	140	0.02%	0.002%
18	3.539	682	684	686	rBV	253	126	0.01%	0.002%
19	3.607	702	705	708	rBV2	182	130	0.02%	0.002%
20	3.626	708	711	714	rVB	234	173	0.02%	0.002%
21	3.710	734	737	743	rVB2	227	243	0.03%	0.003%
22	3.739	743	746	751	rBV2	228	242	0.03%	0.003%
23	3.764	751	754	756	rBV	148	102	0.01%	0.001%
24	3.819	766	771	774	rBV2	221	252	0.03%	0.004%
25	3.870	784	787	790	rBV2	183	170	0.02%	0.002%
26	3.912	796	800	803	rBV	253	232	0.03%	0.003%
27	4.002	824	828	831	rVB	170	144	0.02%	0.002%
28	4.018	831	833	836	rVB2	194	127	0.01%	0.002%
29	4.092	852	856	859	rVV2	220	160	0.02%	0.002%
30	4.153	872	875	878	rBV2	122	94	0.01%	0.001%
31	4.192	883	887	889	rBV	204	129	0.02%	0.002%
32	4.269	909	911	917	rVB2	251	183	0.02%	0.003%
33	4.298	917	920	923	rVB2	191	131	0.02%	0.002%
34	4.459	963	970	972	rBV	184	164	0.02%	0.002%
35	4.485	976	978	981	rVB2	224	150	0.02%	0.002%
36	4.629	1010	1023	1056	rBV2	81730	225240	26.25%	3.171%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050565.D
 Acq On : 31 Aug 2022 21:40
 Operator : SY/MD
 Sample : N4345-01MEDL 400X
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	5.063	1141	1158	1180	rBV2	154398	337969	39.39%	4.759%
38	5.234	1208	1211	1214	rVB2	258	183	0.02%	0.003%
39	5.276	1221	1224	1227	rBV2	588	457	0.05%	0.006%
40	5.366	1249	1252	1254	rBV3	269	151	0.02%	0.002%
41	5.565	1310	1314	1315	rBV	239	124	0.01%	0.002%
42	5.610	1324	1328	1331	rBV2	188	202	0.02%	0.003%
43	5.722	1343	1363	1384	rBV2	318687	858024	100.00%	12.081%
44	5.925	1423	1426	1432	rBV4	419	493	0.06%	0.007%
45	5.986	1440	1445	1448	rBV2	296	303	0.04%	0.004%
46	6.031	1457	1459	1462	rBV2	185	123	0.01%	0.002%
47	6.144	1491	1494	1498	rVB	195	120	0.01%	0.002%
48	6.163	1498	1500	1502	rBV	185	110	0.01%	0.002%
49	6.192	1503	1509	1512	rBV2	209	214	0.02%	0.003%
50	6.250	1512	1527	1557	rBV	280685	540400	62.98%	7.609%
51	6.420	1576	1580	1584	rBV3	216	165	0.02%	0.002%
52	6.626	1642	1644	1650	rBV	139	104	0.01%	0.001%
53	6.690	1650	1664	1690	rBV	200059	393248	45.83%	5.537%
54	6.790	1690	1695	1698	rBV2	385	394	0.05%	0.006%
55	6.851	1712	1714	1718	rBV2	184	127	0.01%	0.002%
56	6.912	1730	1733	1735	rBV2	152	119	0.01%	0.002%
57	7.105	1784	1793	1798	rVB2	282	382	0.04%	0.005%
58	7.160	1808	1810	1812	rBV	161	94	0.01%	0.001%
59	7.198	1817	1822	1825	rVB2	279	259	0.03%	0.004%
60	7.288	1846	1850	1854	rVV2	308	332	0.04%	0.005%
61	7.362	1871	1873	1875	rVV	208	111	0.01%	0.002%
62	7.378	1875	1878	1882	rVV2	292	293	0.03%	0.004%
63	7.565	1924	1936	1955	rBV	87756	156142	18.20%	2.198%
64	7.780	2000	2003	2008	rVB2	172	155	0.02%	0.002%
65	7.899	2026	2040	2066	rBV	366124	644787	75.15%	9.078%
66	8.137	2112	2114	2116	rBV	192	116	0.01%	0.002%
67	8.179	2116	2127	2148	rVV	60604	103083	12.01%	1.451%
68	8.340	2174	2177	2180	rBV2	286	222	0.03%	0.003%
69	8.375	2186	2188	2190	rBV	272	150	0.02%	0.002%
70	8.465	2213	2216	2217	rVB	176	98	0.01%	0.001%
71	8.552	2230	2243	2258	rBV	404855	680064	79.26%	9.575%
72	8.639	2259	2270	2318	rVB2	197761	463769	54.05%	6.530%
73	8.986	2375	2378	2380	rBV2	144	116	0.01%	0.002%
74	9.015	2383	2387	2390	rVB	243	204	0.02%	0.003%
75	9.115	2416	2418	2422	rBV	182	109	0.01%	0.002%
76	9.195	2440	2443	2446	rBV	203	128	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050565.D
 Acq On : 31 Aug 2022 21:40
 Operator : SY/MD
 Sample : N4345-01MEDL 400X
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS1MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	9.230	2451	2454	2457	rBV	224	140	0.02%	0.002%
78	9.291	2469	2473	2480	rBV2	219	281	0.03%	0.004%
79	9.327	2480	2484	2485	rBV	166	116	0.01%	0.002%
80	9.417	2499	2512	2543	rBV	405239	670130	78.10%	9.435%
81	9.732	2605	2610	2612	rBV2	320	248	0.03%	0.003%
82	9.922	2666	2669	2673	rBV2	192	146	0.02%	0.002%
83	9.957	2678	2680	2684	rVB	207	108	0.01%	0.002%
84	10.246	2766	2770	2772	rBV2	248	151	0.02%	0.002%
85	10.381	2806	2812	2818	rBV2	224	410	0.05%	0.006%
86	10.407	2818	2820	2822	rVV2	236	133	0.02%	0.002%
87	10.420	2822	2824	2828	rVB2	310	191	0.02%	0.003%
88	10.484	2842	2844	2848	rVB	217	126	0.01%	0.002%
89	10.671	2900	2902	2904	rBV2	170	92	0.01%	0.001%
90	10.754	2916	2928	2949	rBV	292429	477364	55.64%	6.721%
91	11.092	3031	3033	3037	rVB2	265	168	0.02%	0.002%
92	11.118	3037	3041	3043	rBV2	377	292	0.03%	0.004%
93	11.221	3069	3073	3074	rBV2	366	260	0.03%	0.004%
94	11.606	3190	3193	3196	rBV2	297	216	0.03%	0.003%
95	11.812	3245	3257	3277	rBV	328285	529459	61.71%	7.455%
96	12.192	3362	3375	3398	rBV	327195	545220	63.54%	7.677%
97	12.587	3496	3498	3500	rBV2	300	145	0.02%	0.002%
98	12.915	3597	3600	3602	rBV2	232	136	0.02%	0.002%
99	13.295	3715	3718	3719	rBV2	353	225	0.03%	0.003%
100	13.336	3728	3731	3734	rBV2	413	341	0.04%	0.005%




Sum of corrected areas: 7102371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050565.D
Acq On : 31 Aug 2022 21:40
Operator : SY/MD
Sample : N4345-01MEDL 400X
Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS1MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

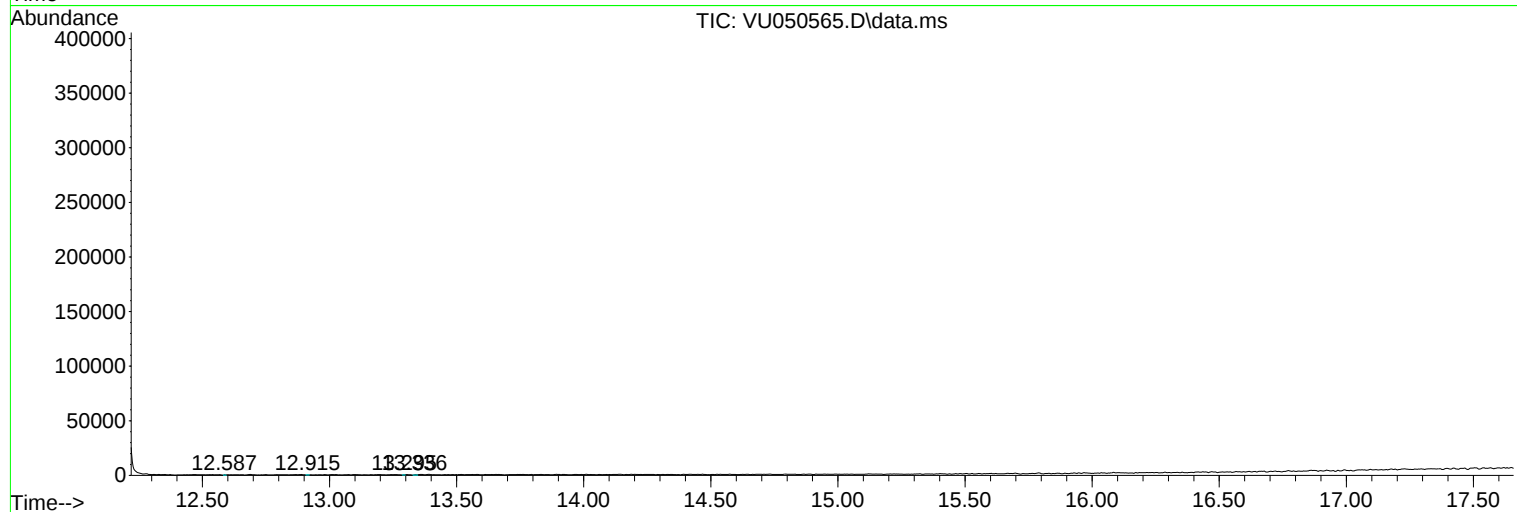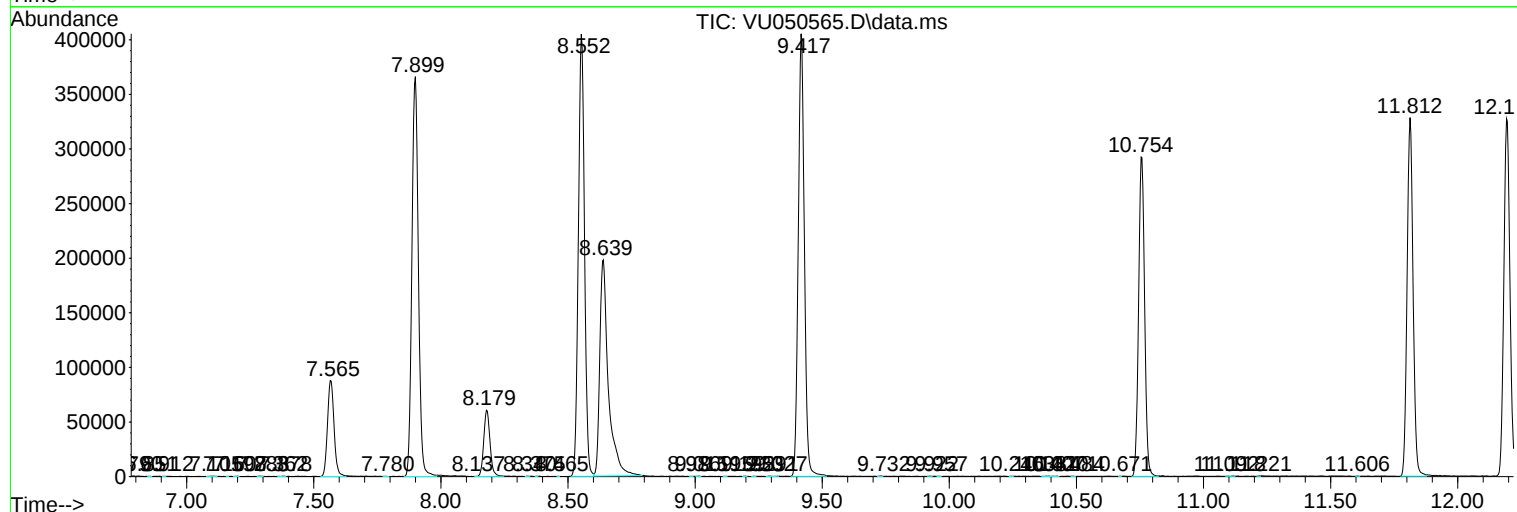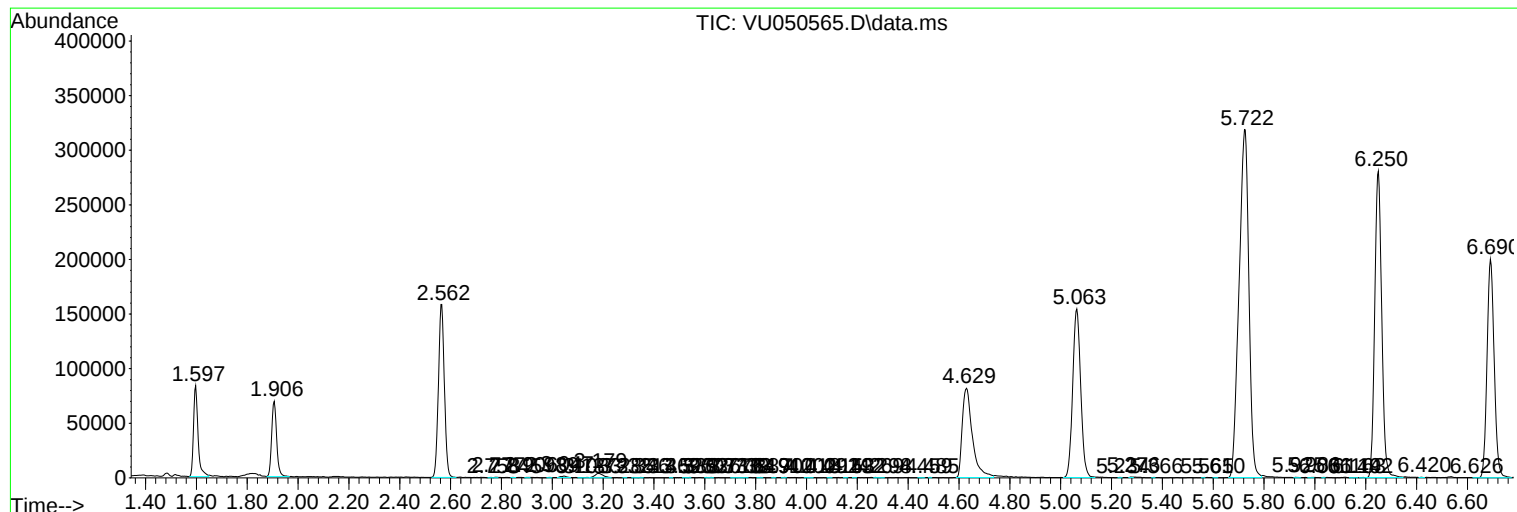

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050565.D
Acq On : 31 Aug 2022 21:40
Operator : SY/MD
Sample : N4345-01MEDL 400X
Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS1MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050565.D
Acq On : 31 Aug 2022 21:40
Operator : SY/MD
Sample : N4345-01MEDL 400X
Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS1MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc