

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050567.D
 Acq On : 31 Aug 2022 22:27
 Operator : SY/MD
 Sample : N4345-02ME 100X
 Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M

Title : VOC Analysis

Signal : TIC: VU050567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	109	rVB	95783	121926	12.10%	1.660%
2	1.765	127	132	133	rBV2	810	588	0.06%	0.008%
3	1.903	167	175	191	rVB	71803	95320	9.46%	1.297%
4	2.186	261	263	266	rBV	420	326	0.03%	0.004%
5	2.311	298	302	303	rBV	458	315	0.03%	0.004%
6	2.324	303	306	309	rVV	309	248	0.02%	0.003%
7	2.366	316	319	325	rVB3	528	540	0.05%	0.007%
8	2.395	325	328	332	rBV2	277	329	0.03%	0.004%
9	2.562	368	380	400	rVV	156329	254403	25.24%	3.463%
10	2.719	424	429	431	rBV	289	279	0.03%	0.004%
11	2.810	455	457	462	rBV2	175	212	0.02%	0.003%
12	3.047	522	531	540	rVB4	1490	2879	0.29%	0.039%
13	3.179	560	572	589	rBV2	4879	11267	1.12%	0.153%
14	3.404	638	642	647	rBV2	179	179	0.02%	0.002%
15	3.488	665	668	673	rVB2	210	199	0.02%	0.003%
16	3.517	673	677	682	rVB2	288	346	0.03%	0.005%
17	3.552	682	688	690	rBV2	204	228	0.02%	0.003%
18	3.629	708	712	715	rBV	290	234	0.02%	0.003%
19	3.678	722	727	730	rBV	312	323	0.03%	0.004%
20	3.912	796	800	803	rVB	265	196	0.02%	0.003%
21	3.938	803	808	810	rBV2	248	257	0.03%	0.003%
22	4.073	848	850	856	rVB	199	172	0.02%	0.002%
23	4.337	928	932	938	rBV	219	270	0.03%	0.004%
24	4.388	944	948	951	rBV	209	191	0.02%	0.003%
25	4.533	991	993	1001	rVB2	245	195	0.02%	0.003%
26	4.629	1007	1023	1065	rBV2	85276	249689	24.77%	3.398%
27	5.006	1135	1140	1142	rBV3	303	314	0.03%	0.004%
28	5.063	1142	1158	1183	rVV	172813	377762	37.48%	5.142%
29	5.279	1222	1225	1227	rBV2	613	460	0.05%	0.006%
30	5.350	1241	1247	1250	rBV2	173	233	0.02%	0.003%
31	5.424	1266	1270	1273	rBV	263	218	0.02%	0.003%
32	5.443	1273	1276	1281	rVV2	193	214	0.02%	0.003%
33	5.581	1316	1319	1323	rBV2	246	274	0.03%	0.004%
34	5.723	1342	1363	1396	rBV2	371799	1007939	100.00%	13.719%
35	6.034	1457	1460	1465	rBV2	318	288	0.03%	0.004%
36	6.108	1477	1483	1484	rBV2	185	196	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050567.D
 Acq On : 31 Aug 2022 22:27
 Operator : SY/MD
 Sample : N4345-02ME 100X
 Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1549	rBV	318500	617897	61.30%	8.410%
38	6.475	1594	1597	1601	rBV2	312	286	0.03%	0.004%
39	6.523	1608	1612	1616	rBV5	896	969	0.10%	0.013%
40	6.565	1623	1625	1631	rVB2	280	228	0.02%	0.003%
41	6.690	1650	1664	1694	rBV	234238	456420	45.28%	6.212%
42	6.883	1719	1724	1728	rBV2	239	206	0.02%	0.003%
43	7.070	1781	1782	1788	rVB2	255	197	0.02%	0.003%
44	7.099	1788	1791	1799	rVB2	246	280	0.03%	0.004%
45	7.182	1814	1817	1819	rBV	282	175	0.02%	0.002%
46	7.253	1834	1839	1843	rBV	355	284	0.03%	0.004%
47	7.565	1923	1936	1953	rBV	97792	175467	17.41%	2.388%
48	7.658	1963	1965	1970	rVB2	654	478	0.05%	0.007%
49	7.690	1971	1975	1977	rBV3	446	311	0.03%	0.004%
50	7.768	1996	1999	2005	rVB2	171	180	0.02%	0.002%
51	7.809	2010	2012	2019	rVB	387	320	0.03%	0.004%
52	7.851	2019	2025	2026	rBV2	282	252	0.03%	0.003%
53	7.899	2026	2040	2071	rBV	425783	739521	73.37%	10.066%
54	8.179	2115	2127	2147	rBV	67487	116893	11.60%	1.591%
55	8.369	2184	2186	2192	rVB3	286	277	0.03%	0.004%
56	8.449	2207	2211	2213	rBV	257	178	0.02%	0.002%
57	8.552	2231	2243	2257	rBV	132435	218856	21.71%	2.979%
58	8.639	2257	2270	2311	rBV4	199231	507974	50.40%	6.914%
59	8.861	2336	2339	2341	rBV2	278	196	0.02%	0.003%
60	8.883	2343	2346	2353	rVV3	345	329	0.03%	0.004%
61	9.005	2381	2384	2387	rVB2	253	197	0.02%	0.003%
62	9.031	2387	2392	2397	rVB	264	261	0.03%	0.004%
63	9.057	2397	2400	2404	rBV2	256	247	0.02%	0.003%
64	9.108	2412	2416	2419	rBV	308	232	0.02%	0.003%
65	9.131	2419	2423	2426	rBV2	445	359	0.04%	0.005%
66	9.230	2448	2454	2457	rBV2	239	274	0.03%	0.004%
67	9.256	2458	2462	2465	rBV	367	384	0.04%	0.005%
68	9.417	2499	2512	2535	rBV	453446	766719	76.07%	10.436%
69	9.864	2644	2651	2654	rBV2	348	426	0.04%	0.006%
70	10.050	2705	2709	2713	rBV2	292	296	0.03%	0.004%
71	10.247	2765	2770	2776	rBV2	300	460	0.05%	0.006%
72	10.536	2856	2860	2865	rBV2	286	332	0.03%	0.005%
73	10.584	2871	2875	2878	rBV2	198	207	0.02%	0.003%
74	10.671	2897	2902	2904	rBV	315	289	0.03%	0.004%
75	10.703	2909	2912	2916	rBV2	238	245	0.02%	0.003%
76	10.755	2916	2928	2953	rBV	319328	515318	51.13%	7.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050567.D
 Acq On : 31 Aug 2022 22:27
 Operator : SY/MD
 Sample : N4345-02ME 100X
 Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.861	2958	2961	2962	rBV2	307	194	0.02%	0.003%
78	10.944	2984	2987	2989	rBV	255	196	0.02%	0.003%
79	11.153	3046	3052	3058	rBV2	305	334	0.03%	0.005%
80	11.346	3110	3112	3118	rVB2	296	245	0.02%	0.003%
81	11.391	3121	3126	3132	rBV	227	309	0.03%	0.004%
82	11.632	3197	3201	3203	rBV2	213	171	0.02%	0.002%
83	11.690	3215	3219	3220	rBV2	276	167	0.02%	0.002%
84	11.735	3229	3233	3235	rBV	195	183	0.02%	0.002%
85	11.812	3243	3257	3278	rBV	335127	542183	53.79%	7.380%
86	12.192	3363	3375	3400	rBV	327820	544937	54.06%	7.417%
87	12.375	3426	3432	3439	rBV2	396	603	0.06%	0.008%
88	12.623	3506	3509	3512	rBV2	311	203	0.02%	0.003%
89	12.726	3540	3541	3544	rVB2	423	172	0.02%	0.002%
90	12.748	3545	3548	3553	rBV	417	344	0.03%	0.005%
91	12.886	3589	3591	3597	rVB2	370	317	0.03%	0.004%
92	12.980	3615	3620	3623	rBV2	493	607	0.06%	0.008%
93	13.272	3708	3711	3713	rBV	313	245	0.02%	0.003%
94	13.314	3721	3724	3726	rBV2	396	284	0.03%	0.004%
95	13.365	3738	3740	3747	rVB2	345	266	0.03%	0.004%
96	14.780	4178	4180	4183	rBV2	317	172	0.02%	0.002%
97	14.906	4217	4219	4223	rBV	302	226	0.02%	0.003%
98	14.941	4228	4230	4233	rBV	366	194	0.02%	0.003%
99	15.687	4460	4462	4466	rBV2	624	425	0.04%	0.006%
100	16.031	4564	4569	4570	rBV3	861	645	0.06%	0.009%




Sum of corrected areas: 7347051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050567.D
Acq On : 31 Aug 2022 22:27
Operator : SY/MD
Sample : N4345-02ME 100X
Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

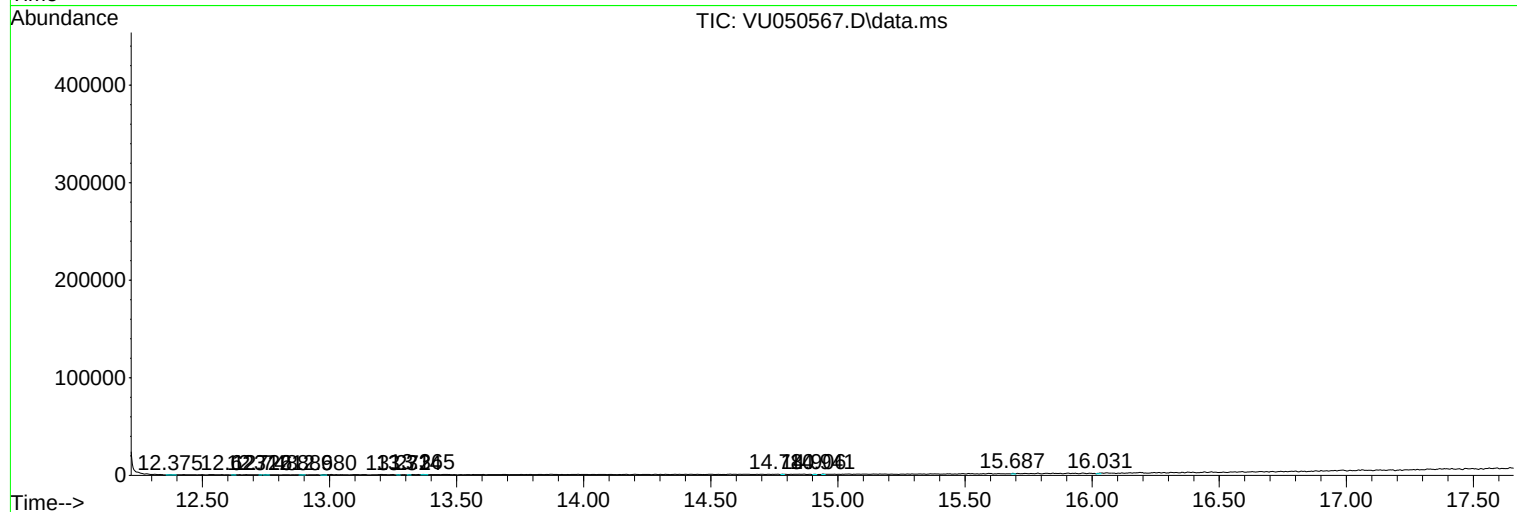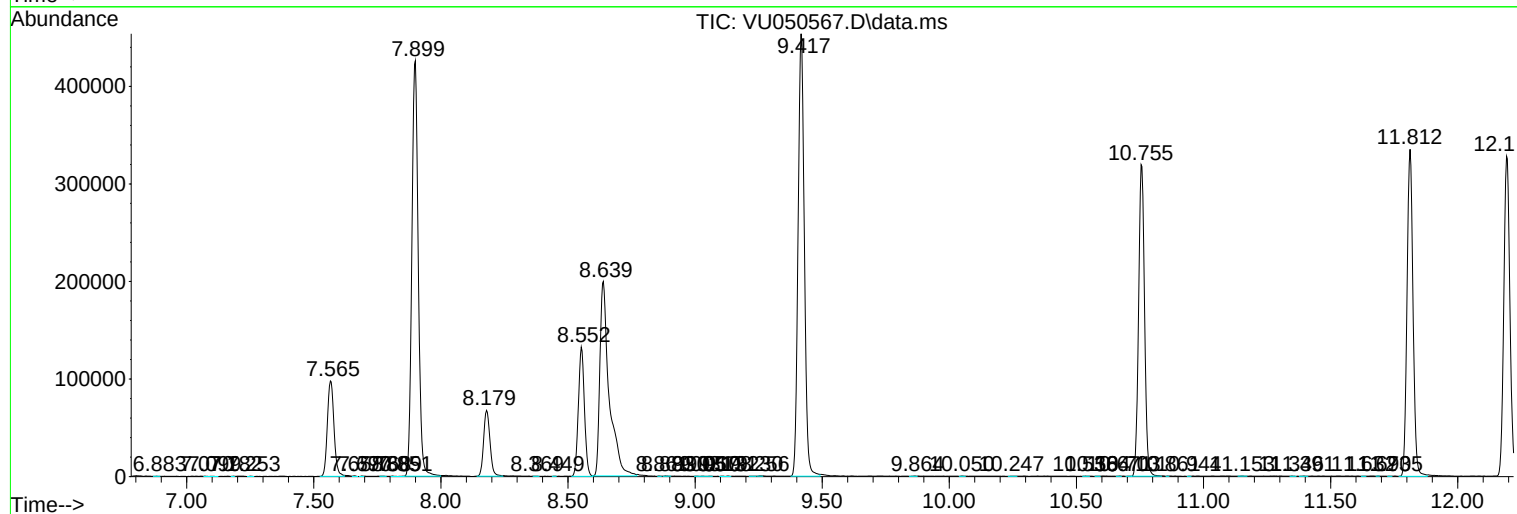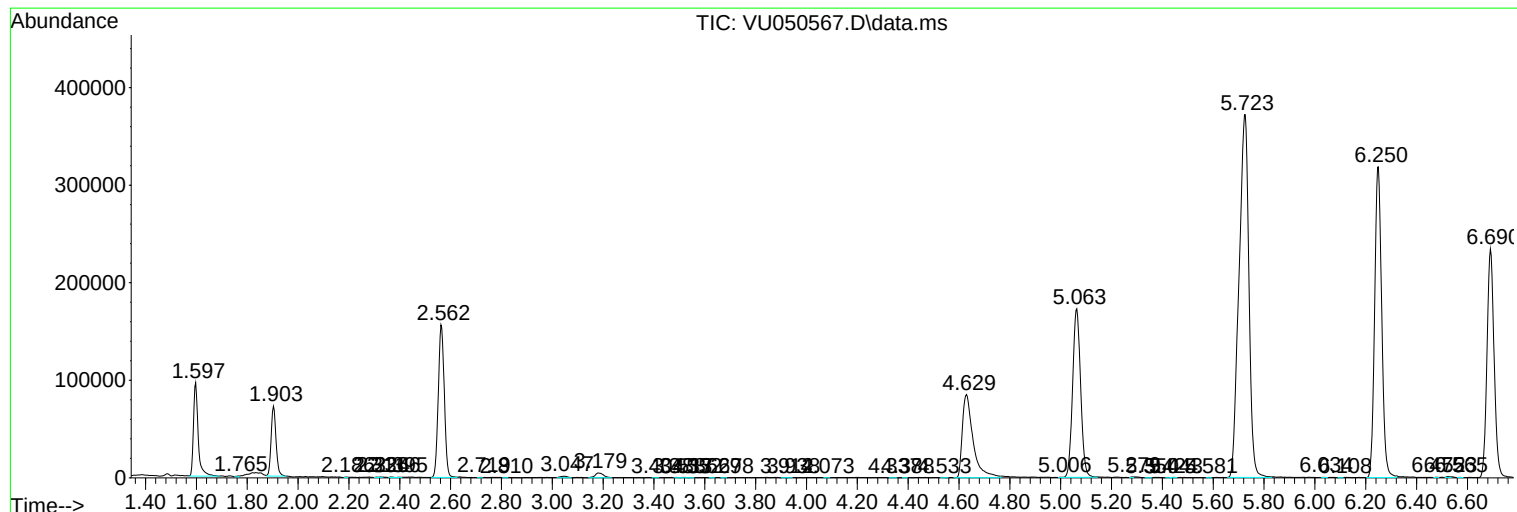

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050567.D
Acq On : 31 Aug 2022 22:27
Operator : SY/MD
Sample : N4345-02ME 100X
Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
Data File : VU050567.D
Acq On : 31 Aug 2022 22:27
Operator : SY/MD
Sample : N4345-02ME 100X
Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc