
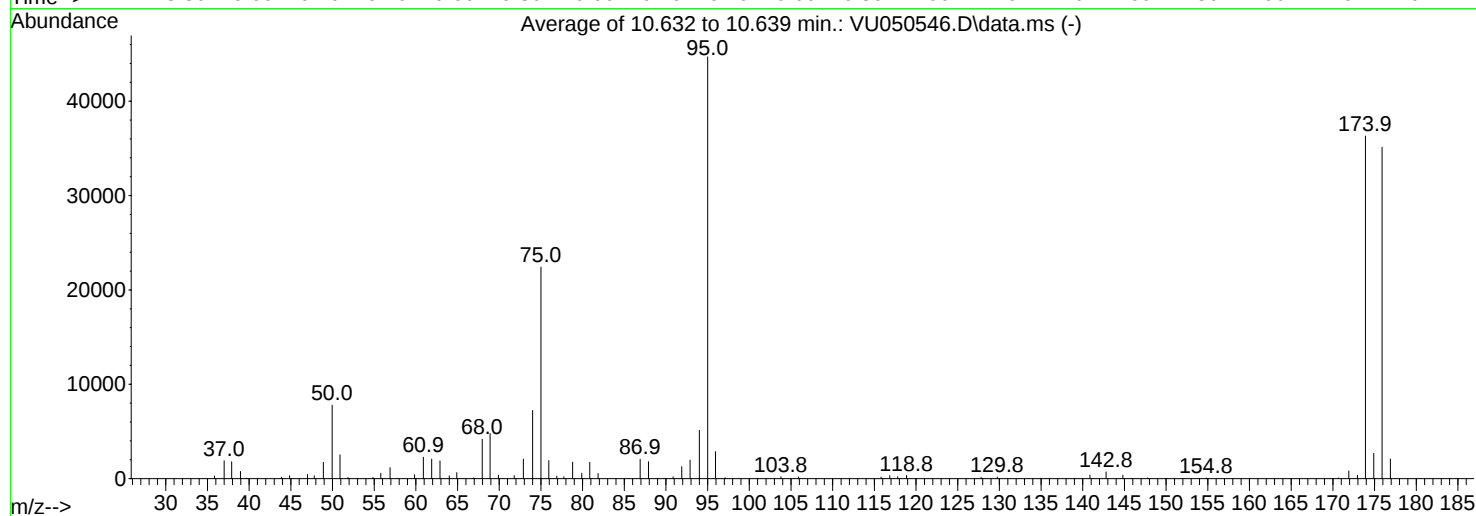


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083122\
 Data File : VU050546.D
 Acq On : 31 Aug 2022 13:26
 Operator : SY/MD
 Sample : BFB116
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB116

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis
 Last Update : Fri Sep 02 02:07:32 2022

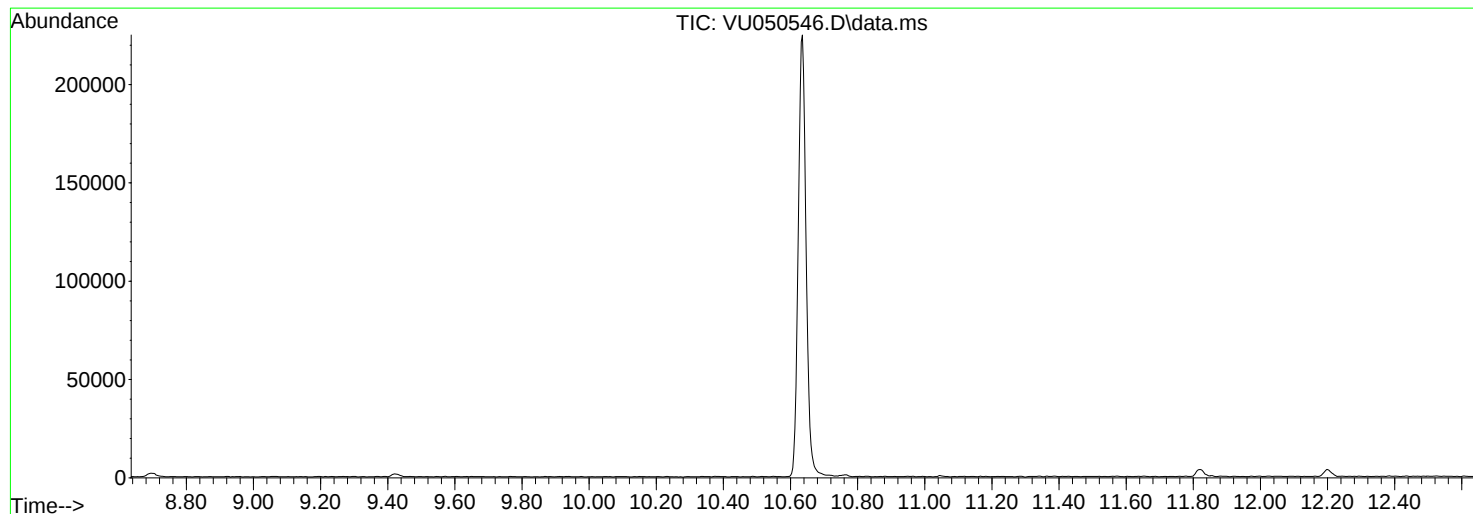

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	7781	PASS
75	95	30	80	50.1	22411	PASS
95	95	100	100	100.0	44704	PASS
96	95	5	9	6.4	2862	PASS
173	174	0.00	2	1.0	364	PASS
174	95	50	120	81.2	36299	PASS
175	174	5	9	7.4	2673	PASS
176	174	95	101	96.7	35112	PASS
177	176	5	9	5.9	2085	PASS

Scan 2878 (10.594 min): VU050546.D\data.ms
BFB116

m/z	Abundance
39.90	198.0
43.90	553.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.90	348.0
37.00	1874.0
37.90	1853.0
38.90	826.0
39.90	180.0
43.90	675.0
44.90	320.0
47.00	499.0
47.80	315.0
48.90	1785.0
50.00	8338.0
50.90	2559.0
51.90	132.0
54.80	134.0
55.80	584.0
56.90	1140.0
57.80	129.0
59.90	455.0
60.90	2522.0
61.90	2227.0
62.90	1914.0
64.00	322.0
64.90	579.0
66.90	127.0
67.90	4462.0
68.90	4905.0
69.90	412.0
71.80	300.0
72.90	2307.0
74.00	7408.0
75.00	22864.0
76.00	1882.0
76.80	290.0
77.70	224.0
78.80	1830.0
79.90	515.0
80.90	1852.0
81.80	556.0
86.90	2166.0
87.90	1666.0
90.90	225.0
91.90	1387.0
92.90	2077.0
94.00	5275.0
95.00	45136.0
95.90	2909.0
97.10	144.0
103.80	197.0
105.90	194.0
115.80	163.0
116.80	331.0
117.80	204.0
118.90	320.0
127.80	108.0
129.80	144.0
140.90	451.0
142.80	687.0
144.80	388.0
147.80	143.0
170.70	115.0
171.90	731.0
173.00	414.0
173.90	36760.0
174.90	2693.0
175.90	34816.0
176.90	2166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.80	295.0
37.00	1963.0
37.90	1834.0
38.90	780.0
40.00	148.0
44.00	706.0
44.80	299.0
47.00	487.0
47.80	323.0
48.90	1767.0
50.00	7994.0
50.90	2620.0
51.90	147.0
54.90	147.0
55.80	594.0
56.90	1203.0
59.80	413.0
60.90	2337.0
61.90	2142.0
62.90	1952.0
64.00	302.0
64.90	657.0
67.00	114.0
67.90	4337.0
68.90	4958.0
69.90	365.0
71.80	347.0
72.90	2114.0
74.00	7482.0
75.00	23328.0
75.90	1979.0
76.90	276.0
77.70	213.0
78.80	1815.0
79.90	601.0
80.90	1745.0
81.80	561.0
86.90	2155.0
87.90	1869.0
90.90	217.0
91.90	1285.0
92.90	2044.0
94.00	5258.0
95.00	46216.0
96.00	2950.0
97.10	139.0
103.80	210.0
105.90	205.0
115.80	173.0
116.80	328.0
117.80	210.0
118.80	347.0
127.80	147.0
129.80	159.0
134.90	113.0
140.80	394.0
142.80	741.0
144.80	398.0
145.70	104.0
147.80	117.0
154.80	104.0
170.70	123.0
171.90	849.0
173.00	365.0
173.90	37456.0
174.90	2776.0
175.90	36248.0
176.90	2121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116

m/z	Abundance
35.80	247.0
37.00	1869.0
37.90	1723.0
39.00	684.0
39.70	140.0
44.00	759.0
44.80	277.0
47.00	354.0
47.80	289.0
48.90	1613.0
49.90	7012.0
50.90	2405.0
51.80	150.0
54.80	154.0
55.80	534.0
56.90	1190.0
59.80	374.0
60.90	1938.0
61.90	1858.0
62.90	1773.0
64.00	284.0
64.90	703.0
68.00	3721.0
68.90	4477.0
69.90	329.0
71.80	319.0
72.90	1790.0
74.00	6761.0
75.00	21040.0
75.90	1892.0
77.00	245.0
77.80	162.0
78.80	1601.0
79.90	596.0
80.80	1596.0
81.90	556.0
86.90	1848.0
87.90	1840.0
90.80	187.0
91.90	1138.0
92.90	1791.0
94.00	4846.0
95.00	42760.0
96.00	2728.0
103.80	184.0
105.90	178.0
115.80	166.0
116.90	309.0
117.80	173.0
118.80	338.0
127.80	167.0
129.70	194.0
140.80	347.0
142.80	718.0
144.80	346.0
154.80	109.0
171.90	871.0
172.80	313.0
173.90	34680.0
174.90	2549.0
175.90	34272.0
176.90	1967.0

Instrument :
MSVOA_U
ClientSampleId :
BFB116