

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055015.D
 Acq On : 31 Aug 2023 12:43
 Operator : MD/SY
 Sample : 04230-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH498

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	24	30	49	rVB2	31925	42307	2.61%	0.592%
2	1.596	88	95	103	rBV	25784	28615	1.76%	0.400%
3	1.904	184	191	204	rVB	38412	52202	3.21%	0.730%
4	2.573	385	399	414	rBV4	134068	260410	16.04%	3.643%
5	3.866	788	801	827	rVB2	27178	68635	4.23%	0.960%
6	4.660	1024	1048	1079	rBV2	610964	1623737	100.00%	22.718%
7	5.078	1157	1178	1199	rBV4	149211	469901	28.94%	6.574%
8	5.525	1301	1317	1329	rBV3	10446	23410	1.44%	0.328%
9	5.721	1357	1378	1395	rBV3	168427	449726	27.70%	6.292%
10	6.245	1527	1541	1560	rBV	203424	394755	24.31%	5.523%
11	6.541	1616	1633	1650	rBV	432328	827787	50.98%	11.582%
12	6.689	1666	1679	1696	rVB	119809	233953	14.41%	3.273%
13	7.566	1941	1952	1968	rBV2	43474	79448	4.89%	1.112%
14	7.898	2043	2055	2075	rBV	198623	352006	21.68%	4.925%
15	8.181	2129	2143	2162	rBV3	26657	46285	2.85%	0.648%
16	8.634	2272	2284	2318	rBV2	282314	630218	38.81%	8.817%
17	9.415	2515	2527	2554	rBV	287411	500778	30.84%	7.006%
18	10.753	2927	2943	2961	rBV	105729	176509	10.87%	2.470%
19	11.811	3260	3272	3289	rBV	304548	486118	29.94%	6.801%
20	12.065	3342	3351	3369	rBV4	10082	22918	1.41%	0.321%
21	12.193	3375	3391	3416	rBV	222579	377732	23.26%	5.285%




Sum of corrected areas: 7147450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055015.D
Acq On : 31 Aug 2023 12:43
Operator : MD/SY
Sample : 04230-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH498

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

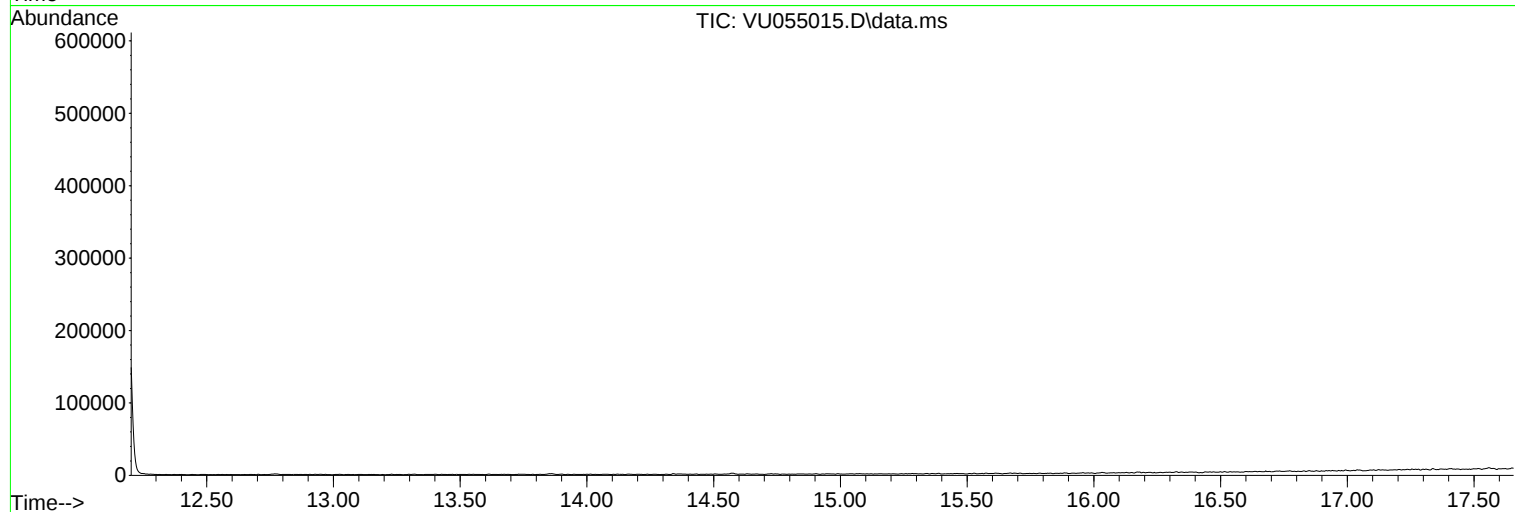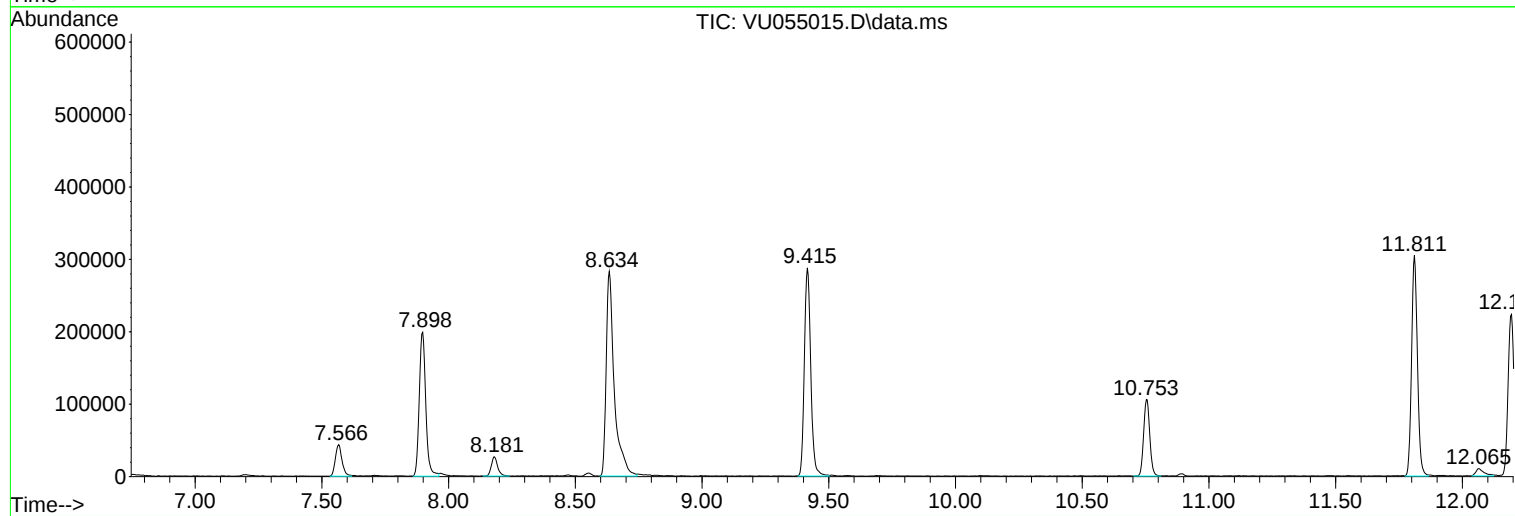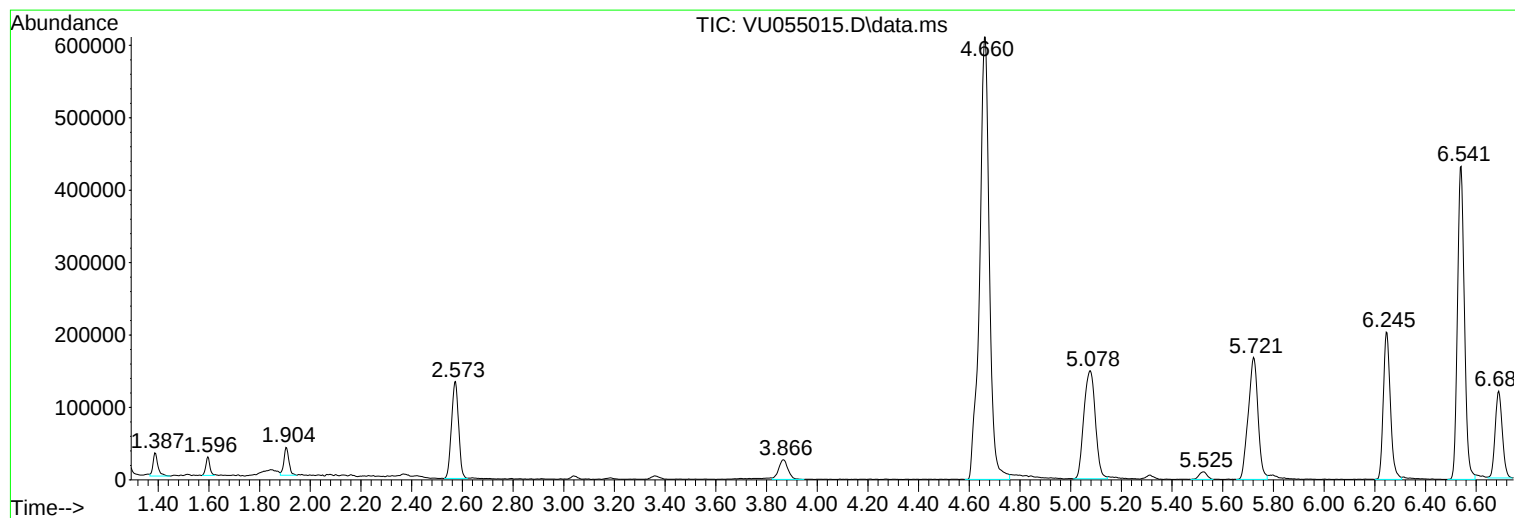

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055015.D
Acq On : 31 Aug 2023 12:43
Operator : MD/SY
Sample : 04230-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH498

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055015.D
Acq On : 31 Aug 2023 12:43
Operator : MD/SY
Sample : 04230-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH498

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc