

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055018.D
 Acq On : 31 Aug 2023 13:58
 Operator : MD/SY
 Sample : 04153-08 2500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH476

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	106	rVB	51189	59345	10.89%	1.275%
2	1.907	184	192	210	rVB	68708	94246	17.29%	2.024%
3	2.560	383	395	411	rBV	113507	186837	34.28%	4.013%
4	3.042	532	545	562	rBV3	14751	28002	5.14%	0.601%
5	3.181	575	588	603	rVB2	7994	18956	3.48%	0.407%
6	4.631	1025	1039	1072	rBV	76724	226146	41.49%	4.857%
7	5.062	1155	1173	1197	rBV	102189	234973	43.11%	5.046%
8	5.724	1359	1379	1399	rBV2	208597	545039	100.00%	11.705%
9	6.248	1527	1542	1564	rBV	194594	382613	70.20%	8.217%
10	6.541	1619	1633	1647	rBV10	10461	23564	4.32%	0.506%
11	6.688	1666	1679	1701	rBV	131179	264228	48.48%	5.675%
12	7.563	1940	1951	1971	rBV2	50021	92972	17.06%	1.997%
13	7.897	2040	2055	2076	rBV	251526	456444	83.75%	9.803%
14	8.180	2129	2143	2157	rBV2	28485	51122	9.38%	1.098%
15	8.634	2273	2284	2318	rBV3	219811	493275	90.50%	10.594%
16	9.415	2515	2527	2549	rBV	272545	474051	86.98%	10.181%
17	10.753	2931	2943	2958	rBV	92031	150862	27.68%	3.240%
18	11.810	3260	3272	3292	rBV	291261	481148	88.28%	10.333%
19	12.193	3378	3391	3412	rBV2	232295	392472	72.01%	8.429%




Sum of corrected areas: 4656295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055018.D
Acq On : 31 Aug 2023 13:58
Operator : MD/SY
Sample : 04153-08 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH476

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

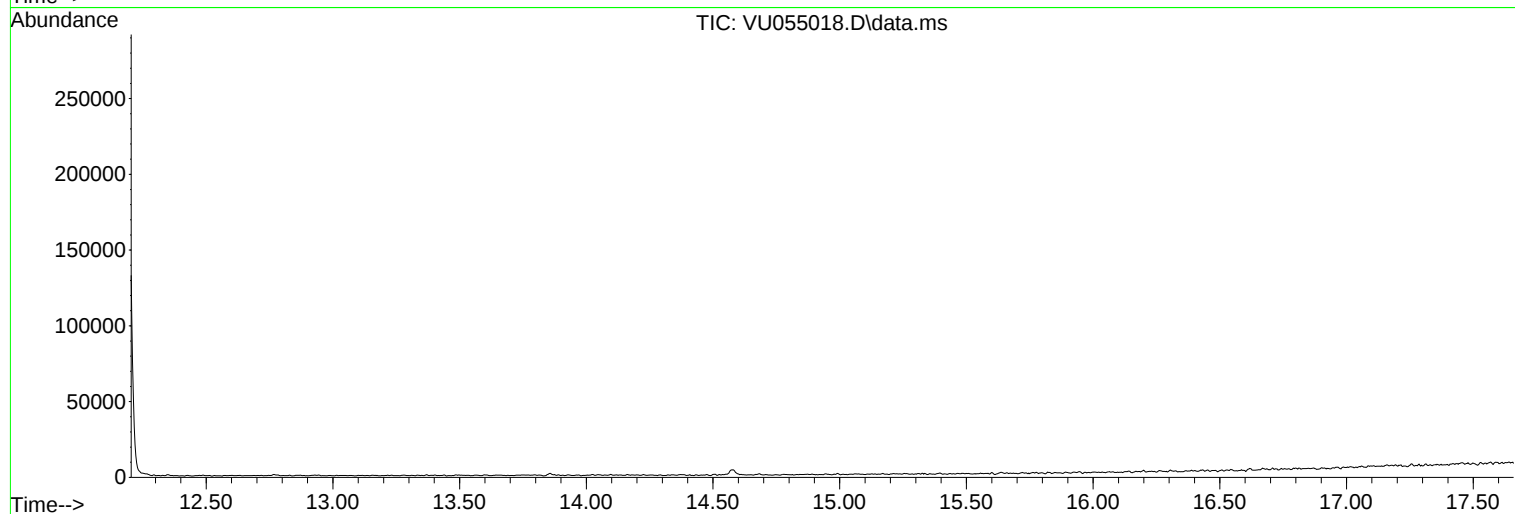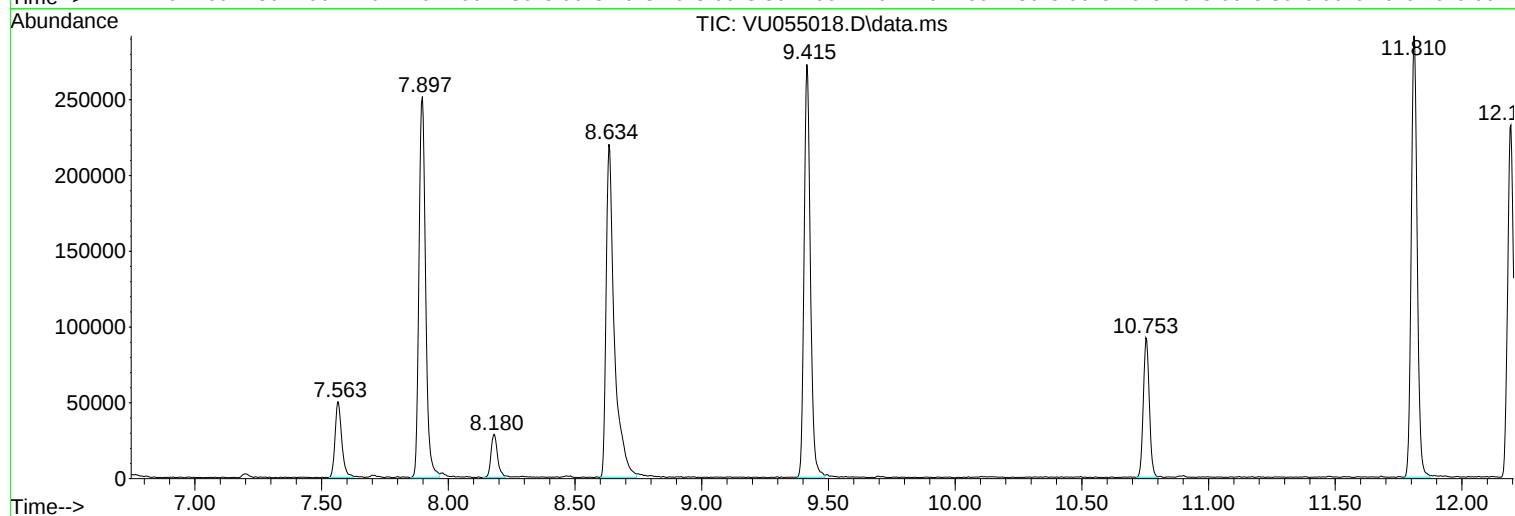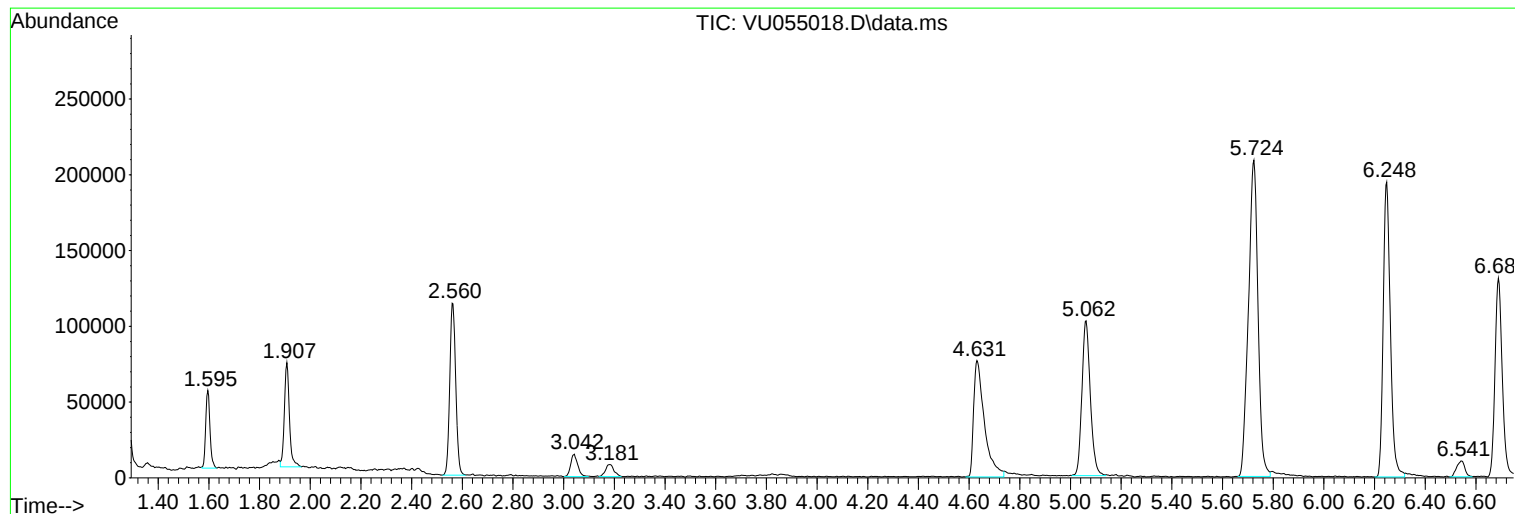

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055018.D
Acq On : 31 Aug 2023 13:58
Operator : MD/SY
Sample : 04153-08 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH476

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055018.D
Acq On : 31 Aug 2023 13:58
Operator : MD/SY
Sample : 04153-08 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH476

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc