

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055019.D
 Acq On : 31 Aug 2023 14:22
 Operator : MD/SY
 Sample : 04153-09 2500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH477

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rBV	53628	63926	11.34%	1.327%
2	1.907	184	192	208	rVB	70389	96889	17.19%	2.012%
3	2.560	384	395	411	rBV	114597	191252	33.92%	3.971%
4	3.039	533	544	563	rVB2	23939	45194	8.02%	0.938%
5	3.184	576	589	597	rBV3	3172	6132	1.09%	0.127%
6	4.631	1028	1039	1066	rBV2	77074	210383	37.32%	4.368%
7	5.058	1156	1172	1192	rBV2	104970	238788	42.36%	4.958%
8	5.721	1360	1378	1402	rBV2	215275	563770	100.00%	11.706%
9	6.248	1528	1542	1564	rBV2	206241	402862	71.46%	8.365%
10	6.534	1618	1631	1646	rBV8	9653	21314	3.78%	0.443%
11	6.689	1664	1679	1698	rBV2	137539	273271	48.47%	5.674%
12	7.566	1939	1952	1970	rBV	50466	94268	16.72%	1.957%
13	7.898	2038	2055	2083	rBV	264026	473261	83.95%	9.827%
14	8.180	2132	2143	2159	rBV	28485	51601	9.15%	1.071%
15	8.634	2270	2284	2320	rBV3	230590	523628	92.88%	10.873%
16	9.415	2515	2527	2554	rBV	291699	502154	89.07%	10.427%
17	10.753	2932	2943	2967	rVB	95014	157958	28.02%	3.280%
18	11.811	3259	3272	3290	rBV	300487	495490	87.89%	10.288%
19	12.190	3375	3390	3411	rBV	239001	403882	71.64%	8.386%




Sum of corrected areas: 4816023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055019.D
Acq On : 31 Aug 2023 14:22
Operator : MD/SY
Sample : 04153-09 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH477

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

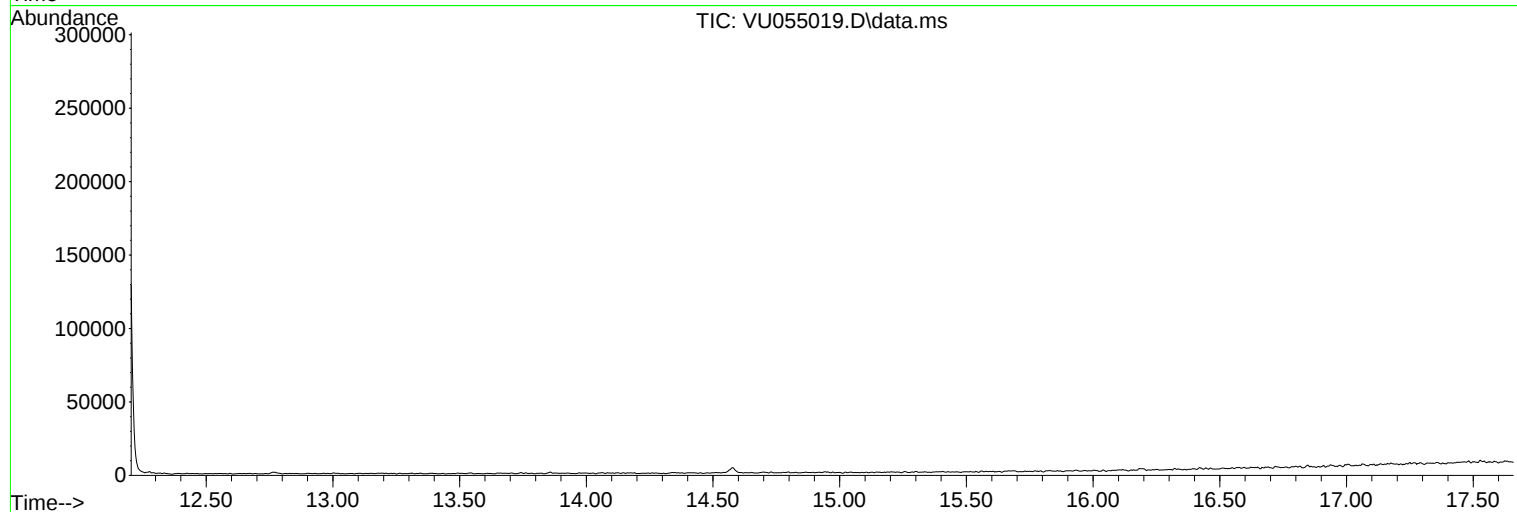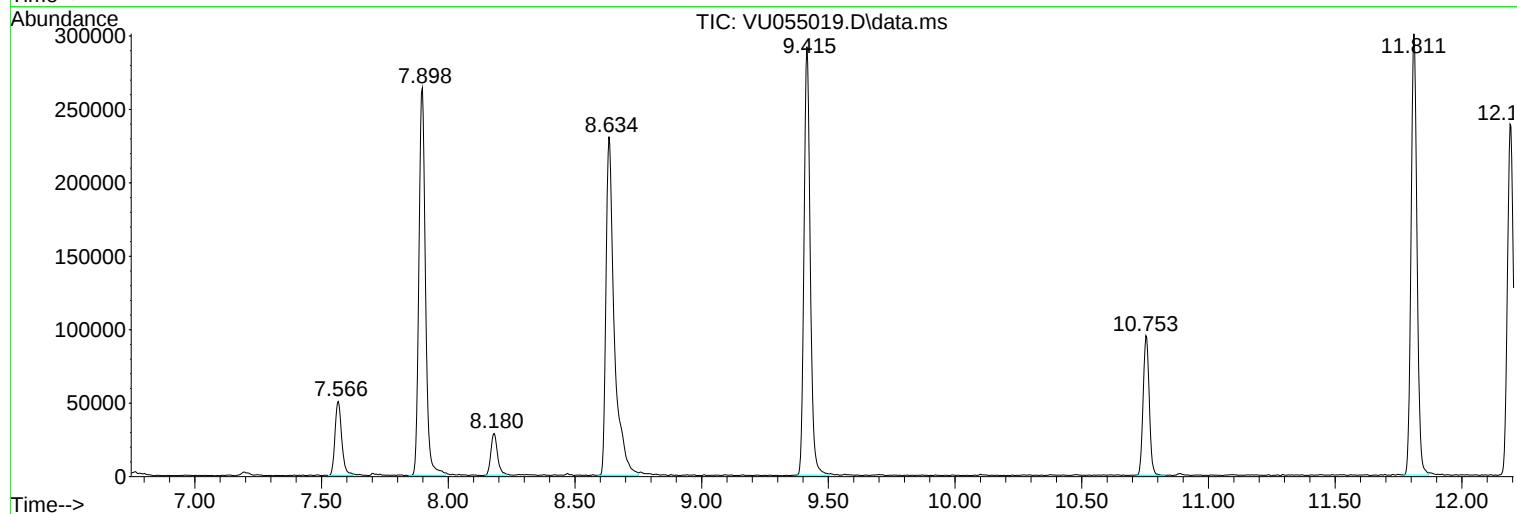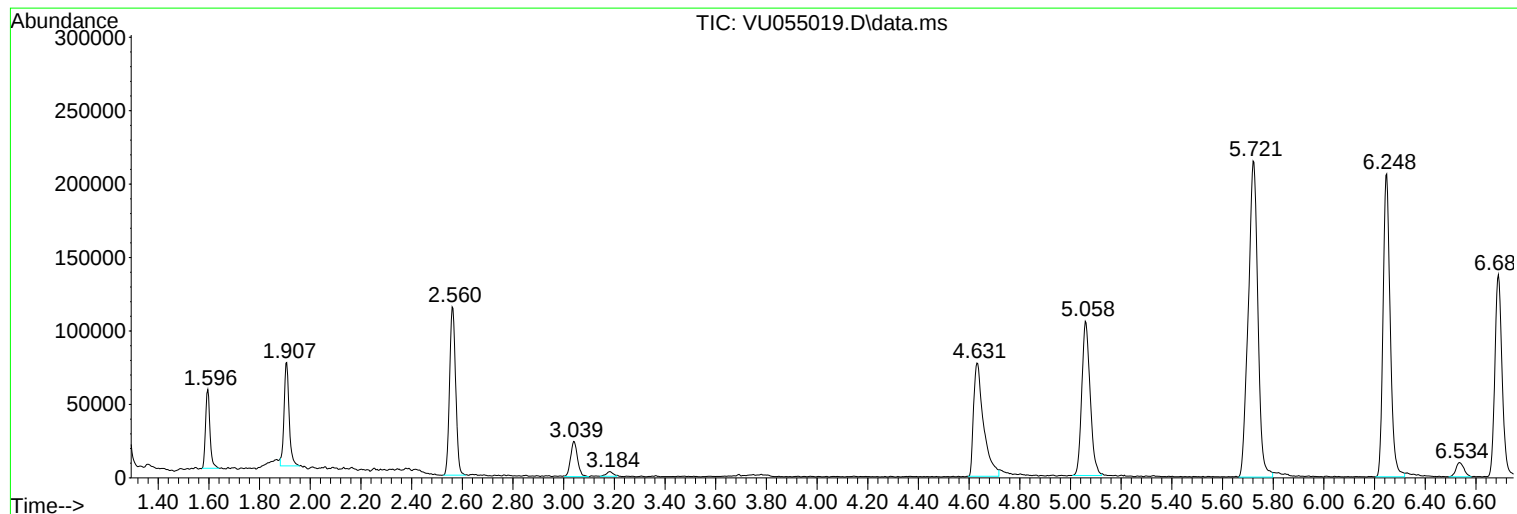

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055019.D
Acq On : 31 Aug 2023 14:22
Operator : MD/SY
Sample : 04153-09 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH477

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055019.D
Acq On : 31 Aug 2023 14:22
Operator : MD/SY
Sample : 04153-09 2500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH477

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------