

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055023.D
 Acq On : 31 Aug 2023 16:00
 Operator : MD/SY
 Sample : 04209-21DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH489DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	106	rBV	55817	65850	10.46%	1.051%
2	1.908	184	192	206	rVB	74753	102158	16.23%	1.631%
3	2.560	382	395	409	rBV	124857	205901	32.71%	3.287%
4	3.039	534	544	559	rVB3	17302	31159	4.95%	0.497%
5	3.184	574	589	608	rVB	27408	63118	10.03%	1.007%
6	4.657	1025	1047	1074	rBV4	138773	535576	85.07%	8.549%
7	5.062	1156	1173	1195	rBV	118322	266405	42.32%	4.252%
8	5.724	1358	1379	1398	rBV3	236327	606551	96.35%	9.682%
9	6.248	1528	1542	1561	rBV	237094	464154	73.73%	7.409%
10	6.541	1620	1633	1651	rBV	268225	514443	81.72%	8.211%
11	6.689	1665	1679	1698	rBV	148060	288432	45.82%	4.604%
12	7.566	1939	1952	1971	rBV	55961	104900	16.66%	1.674%
13	7.894	2038	2054	2074	rBV	284586	511368	81.23%	8.162%
14	8.181	2132	2143	2161	rBV	32033	57824	9.19%	0.923%
15	8.554	2249	2259	2269	rBV4	12886	21511	3.42%	0.343%
16	8.634	2273	2284	2315	rBV2	258651	564926	89.74%	9.017%
17	9.415	2515	2527	2553	rBV	357724	616464	97.92%	9.840%
18	10.756	2931	2944	2960	rBV	103281	171759	27.28%	2.742%
19	11.811	3260	3272	3299	rBV	386151	629546	100.00%	10.049%
20	12.193	3377	3391	3410	rBV	269594	442966	70.36%	7.070%




Sum of corrected areas: 6265011

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055023.D
Acq On : 31 Aug 2023 16:00
Operator : MD/SY
Sample : 04209-21DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH489DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

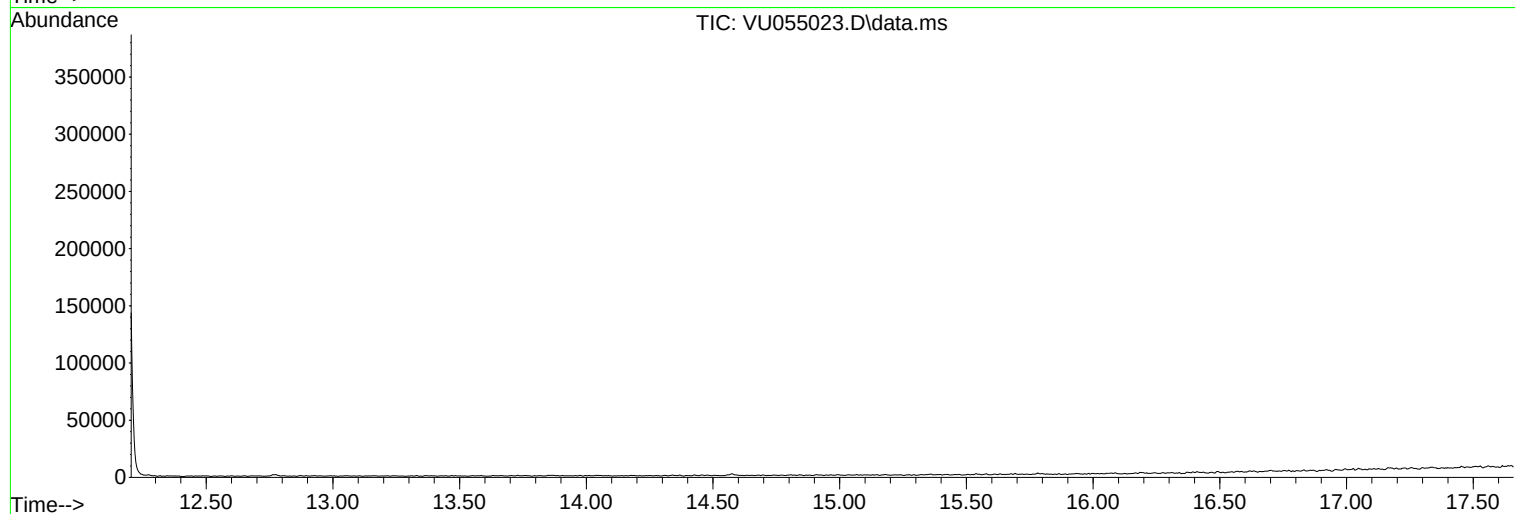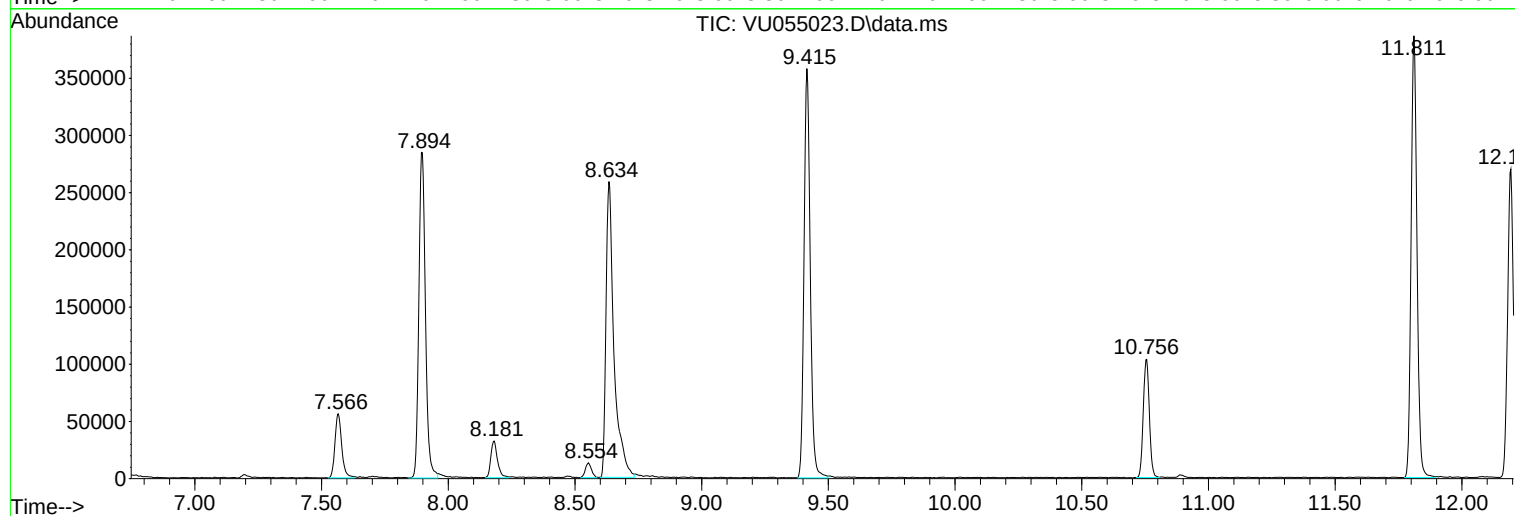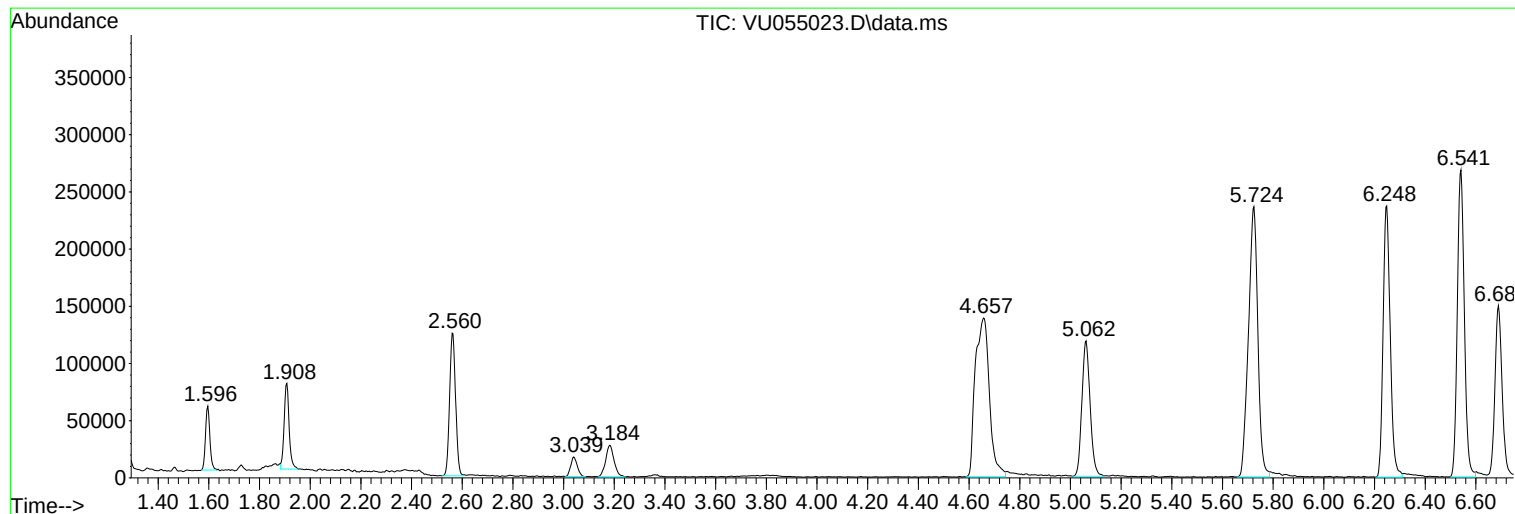

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055023.D
Acq On : 31 Aug 2023 16:00
Operator : MD/SY
Sample : 04209-21DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH489DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055023.D
Acq On : 31 Aug 2023 16:00
Operator : MD/SY
Sample : 04209-21DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH489DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc