

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055026.D
 Acq On : 31 Aug 2023 17:14
 Operator : MD/SY
 Sample : 04230-01DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH490DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rVB	52428	61168	6.93%	0.988%
2	1.904	184	191	204	rVB	67273	88265	9.99%	1.426%
3	2.560	382	395	412	rBV2	117693	191800	21.72%	3.099%
4	3.039	533	544	558	rVB2	16788	30713	3.48%	0.496%
5	3.184	574	589	604	rBV2	21101	47914	5.42%	0.774%
6	4.663	1025	1049	1080	rBV3	293548	883242	100.00%	14.271%
7	5.062	1155	1173	1196	rBV	107098	240303	27.21%	3.883%
8	5.724	1355	1379	1399	rBV2	212866	554900	62.83%	8.966%
9	6.245	1529	1541	1563	rBV	244025	477545	54.07%	7.716%
10	6.541	1620	1633	1650	rBV	207116	396837	44.93%	6.412%
11	6.689	1666	1679	1695	rBV2	133250	261618	29.62%	4.227%
12	7.566	1940	1952	1971	rBV2	52940	95799	10.85%	1.548%
13	7.898	2039	2055	2077	rBV	262965	461420	52.24%	7.455%
14	8.181	2133	2143	2164	rBV	30170	54694	6.19%	0.884%
15	8.553	2248	2259	2269	rVB7	9173	15523	1.76%	0.251%
16	8.634	2269	2284	2319	rBV2	231815	515510	58.37%	8.329%
17	9.415	2515	2527	2551	rBV	362801	618658	70.04%	9.996%
18	10.756	2933	2944	2966	rBV	96108	155749	17.63%	2.516%
19	11.811	3259	3272	3294	rBV	395856	634088	71.79%	10.245%
20	12.193	3379	3391	3408	rBV	245221	403435	45.68%	6.518%




Sum of corrected areas: 6189181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055026.D
Acq On : 31 Aug 2023 17:14
Operator : MD/SY
Sample : 04230-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH490DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

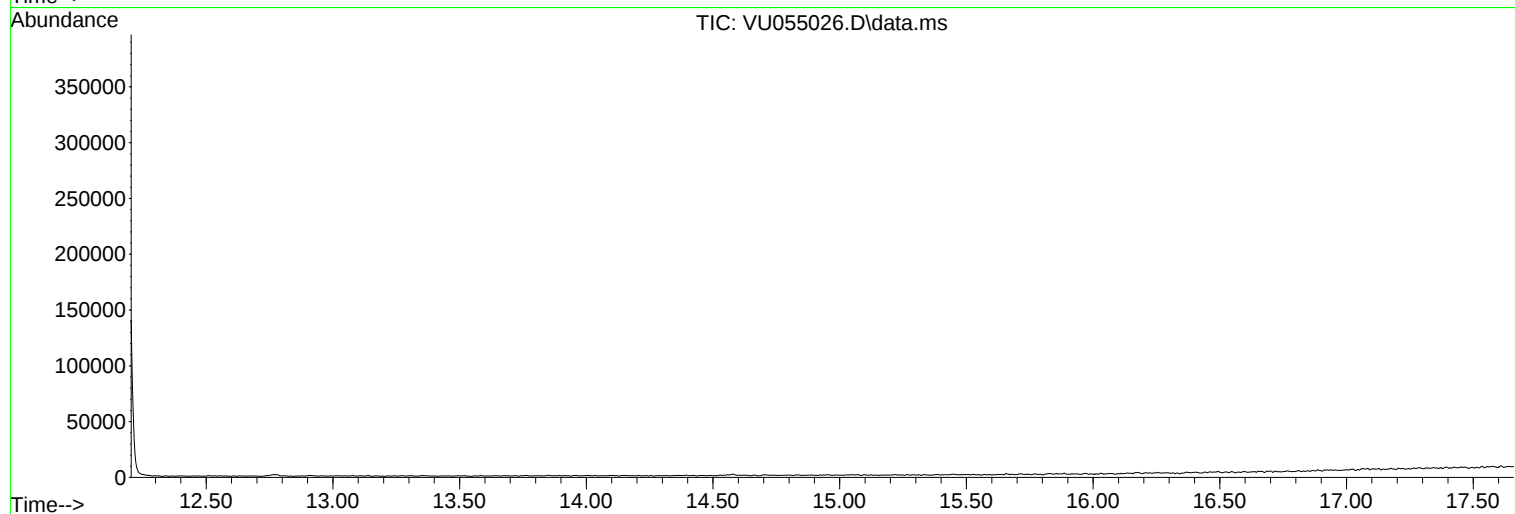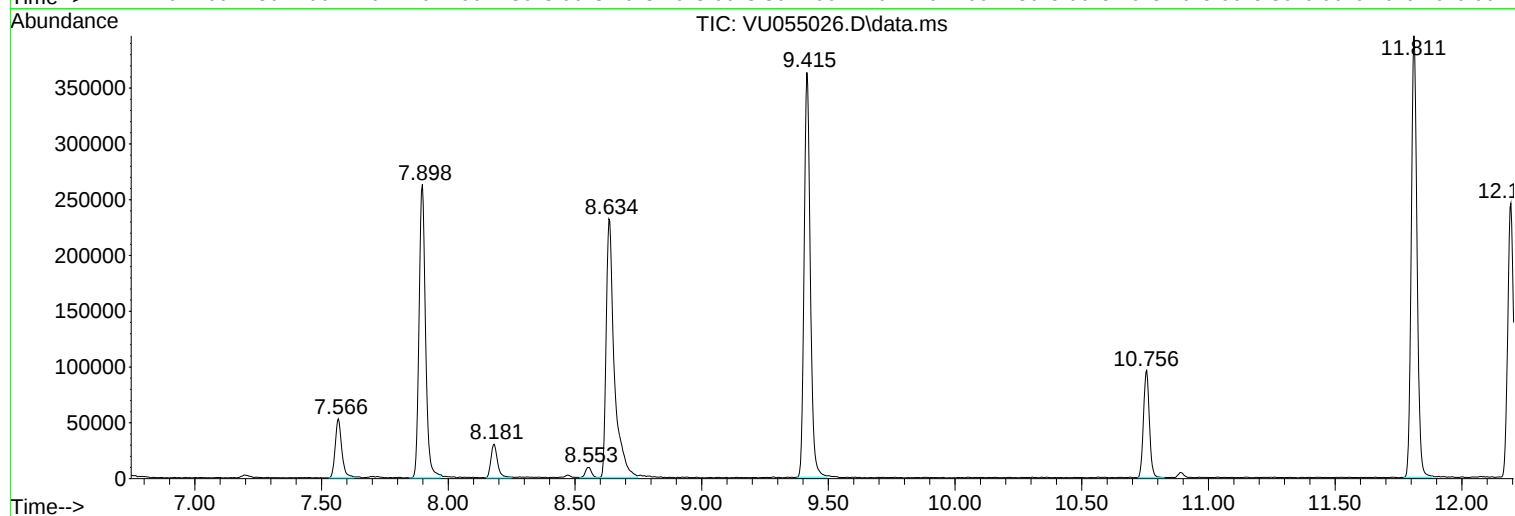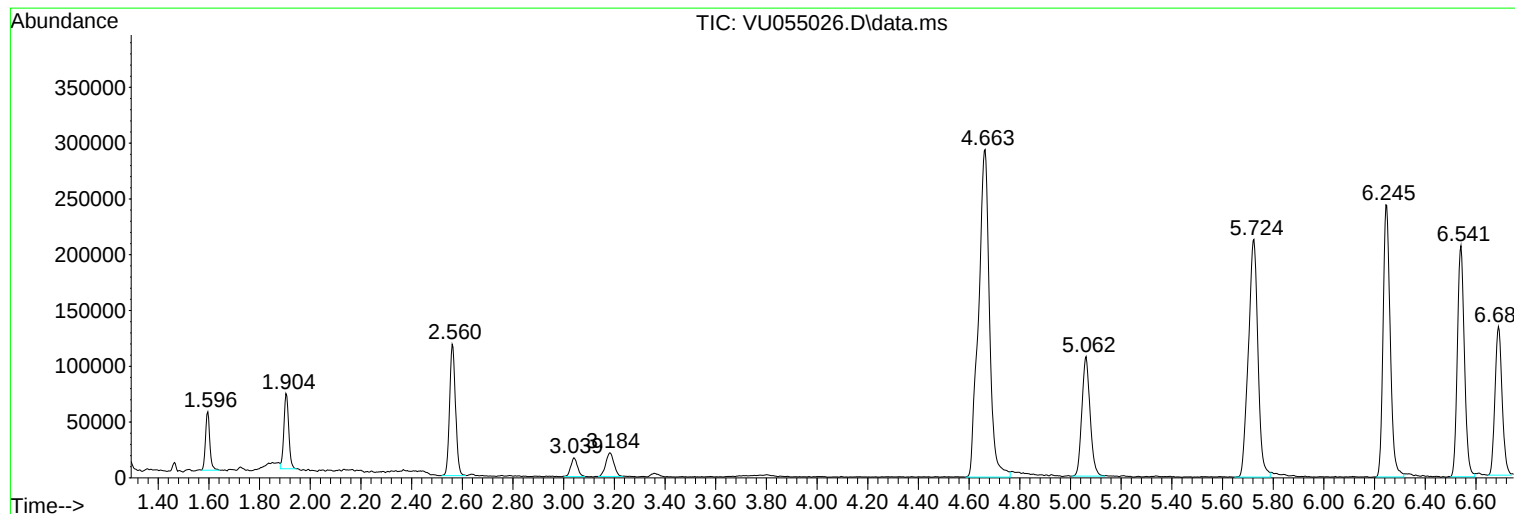

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055026.D
Acq On : 31 Aug 2023 17:14
Operator : MD/SY
Sample : 04230-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH490DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055026.D
Acq On : 31 Aug 2023 17:14
Operator : MD/SY
Sample : 04230-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH490DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc