

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055027.D
 Acq On : 31 Aug 2023 17:39
 Operator : MD/SY
 Sample : 04230-02DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH491DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	109	rBV	51853	60265	9.46%	1.034%
2	1.904	184	191	204	rVB	63000	86587	13.59%	1.486%
3	2.560	380	395	411	rBV	114915	189654	29.77%	3.255%
4	3.042	533	545	560	rBV	32597	63253	9.93%	1.086%
5	3.184	574	589	603	rBV2	9494	21894	3.44%	0.376%
6	4.660	1024	1048	1072	rBV3	173144	572980	89.95%	9.835%
7	5.062	1154	1173	1195	rBV2	103847	239642	37.62%	4.113%
8	5.724	1355	1379	1400	rBV2	212864	551734	86.61%	9.470%
9	6.248	1528	1542	1562	rBV	243301	473323	74.30%	8.124%
10	6.541	1620	1633	1661	rBV	192748	375966	59.02%	6.453%
11	6.688	1666	1679	1697	rVV	134098	260306	40.86%	4.468%
12	7.566	1941	1952	1970	rBV	50313	91161	14.31%	1.565%
13	7.897	2042	2055	2073	rBV	256774	454009	71.27%	7.793%
14	8.180	2132	2143	2158	rBV	29754	50804	7.98%	0.872%
15	8.634	2272	2284	2318	rBV2	223893	514571	80.78%	8.832%
16	9.415	2515	2527	2554	rBV	361351	623981	97.96%	10.710%
17	10.753	2932	2943	2962	rBV	95253	156594	24.58%	2.688%
18	11.810	3256	3272	3292	rBV	391975	637005	100.00%	10.933%
19	12.193	3372	3391	3411	rBV	238250	402470	63.18%	6.908%




Sum of corrected areas: 5826199

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055027.D
Acq On : 31 Aug 2023 17:39
Operator : MD/SY
Sample : 04230-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH491DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

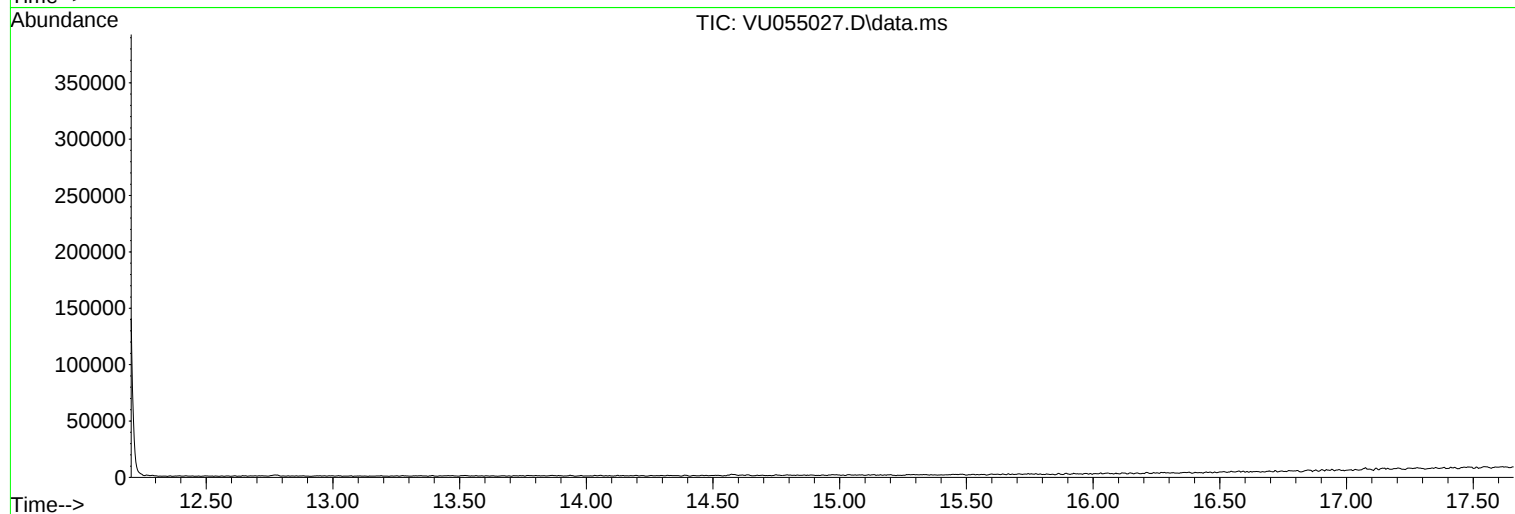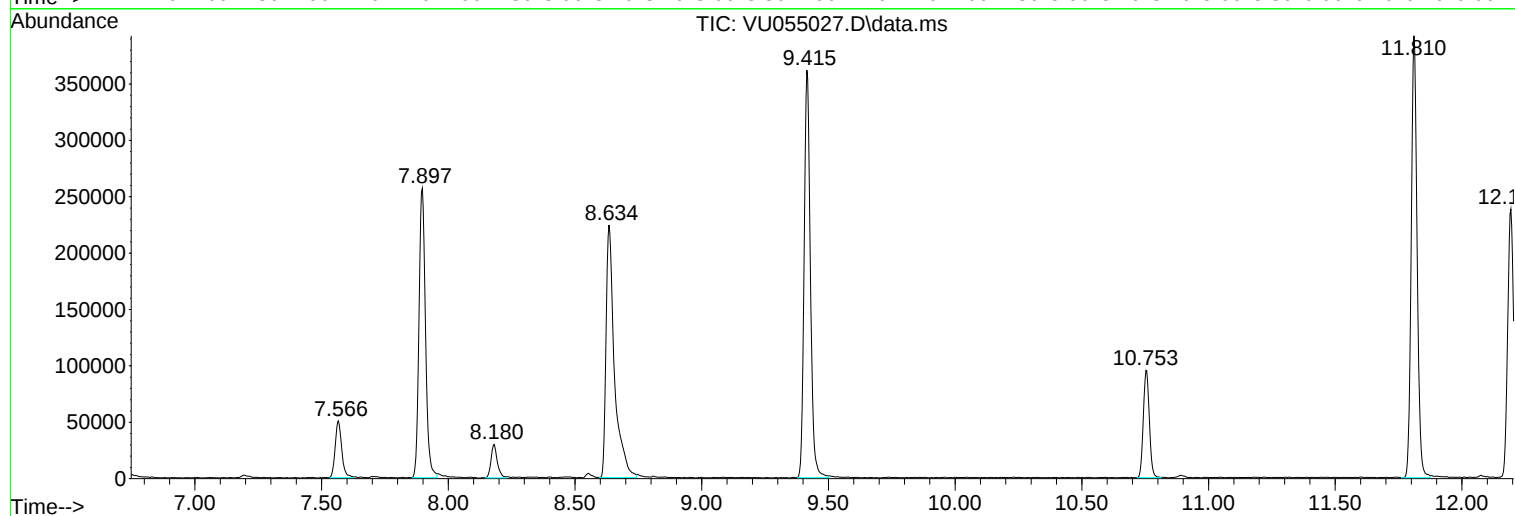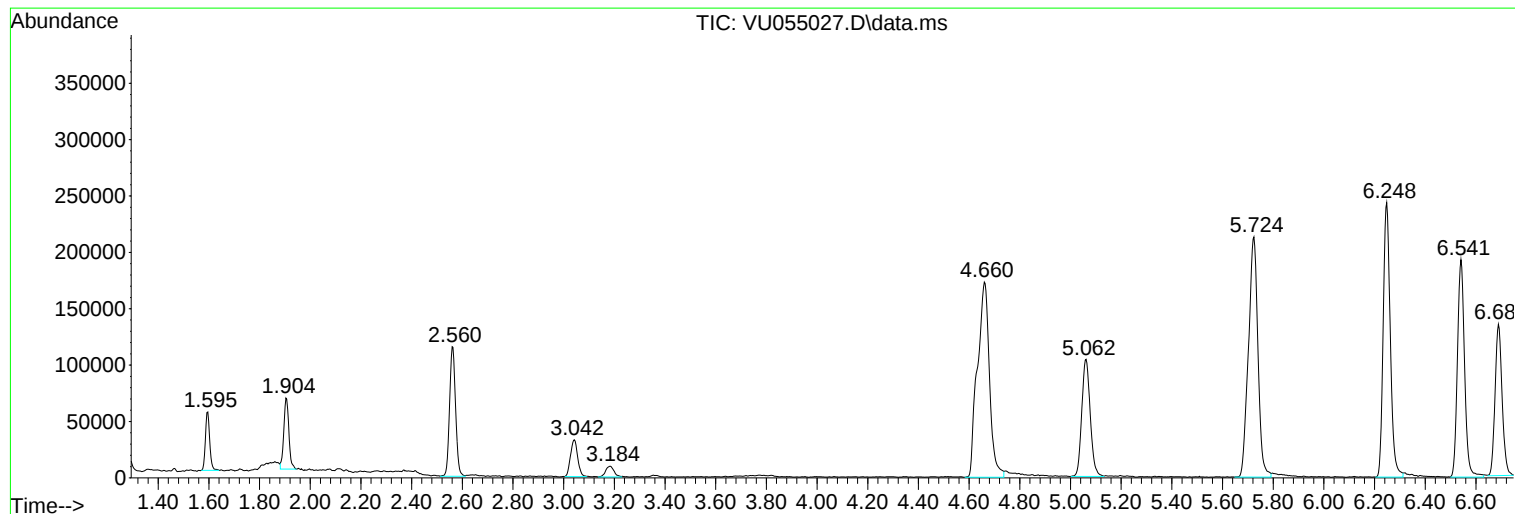

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055027.D
Acq On : 31 Aug 2023 17:39
Operator : MD/SY
Sample : 04230-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH491DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055027.D
Acq On : 31 Aug 2023 17:39
Operator : MD/SY
Sample : 04230-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH491DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc