

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
 Data File : VU055032.D
 Acq On : 31 Aug 2023 19:42
 Operator : MD/SY
 Sample : 04153-06 1000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH464

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	109	rVB	53338	61658	5.60%	0.864%
2	1.907	185	192	204	rVB	66011	83627	7.60%	1.172%
3	2.563	384	396	411	rBV	112030	186481	16.94%	2.614%
4	3.039	531	544	568	rBV	196119	371413	33.74%	5.206%
5	3.181	573	588	606	rVV	37943	88528	8.04%	1.241%
6	4.660	1021	1048	1072	rBV2	240053	757533	68.82%	10.619%
7	5.062	1157	1173	1196	rBV	102777	234344	21.29%	3.285%
8	5.721	1357	1378	1400	rBV4	211705	554023	50.33%	7.766%
9	6.248	1527	1542	1564	rBV	251251	490177	44.53%	6.871%
10	6.541	1614	1633	1660	rBV	571741	1100771	100.00%	15.430%
11	6.689	1667	1679	1697	rVB	132475	262596	23.86%	3.681%
12	7.566	1939	1952	1969	rBV2	49790	92209	8.38%	1.293%
13	7.898	2042	2055	2082	rBV	257052	461976	41.97%	6.476%
14	8.180	2131	2143	2157	rBV3	27258	49387	4.49%	0.692%
15	8.634	2273	2284	2320	rVV3	219674	499845	45.41%	7.007%
16	9.415	2514	2527	2555	rBV	367297	634933	57.68%	8.900%
17	10.753	2928	2943	2956	rBV	90262	149511	13.58%	2.096%
18	11.811	3260	3272	3292	rBV	404522	657885	59.77%	9.222%
19	12.193	3378	3391	3413	rBV	236645	396930	36.06%	5.564%




Sum of corrected areas: 7133827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055032.D
Acq On : 31 Aug 2023 19:42
Operator : MD/SY
Sample : 04153-06 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH464

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

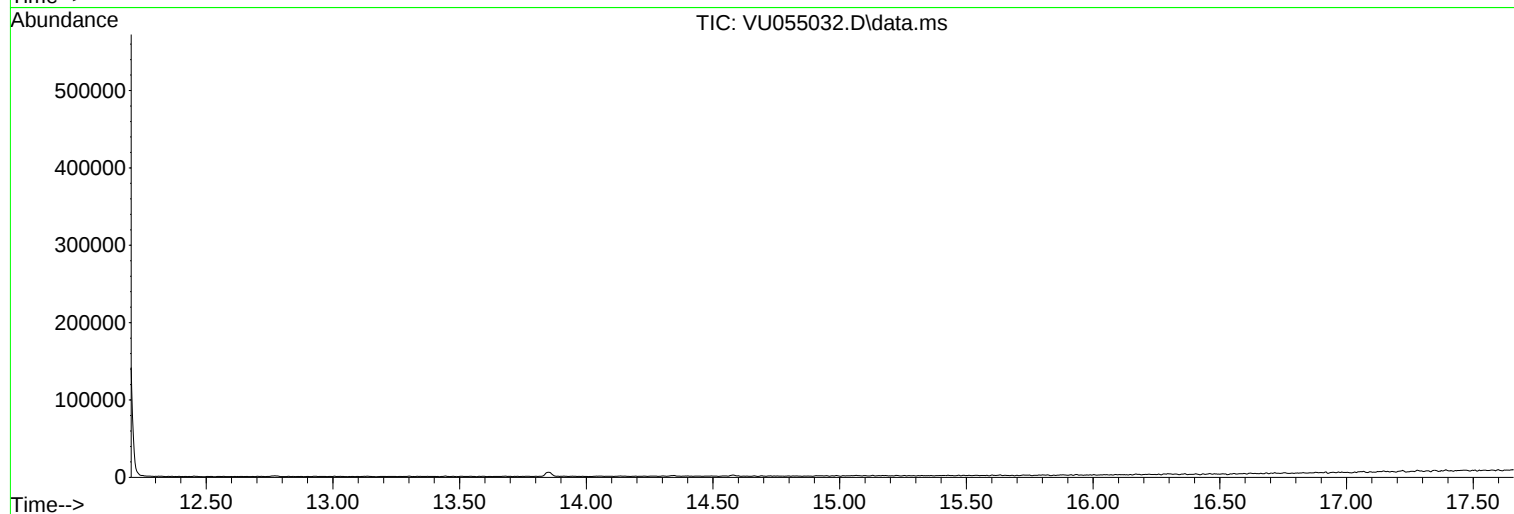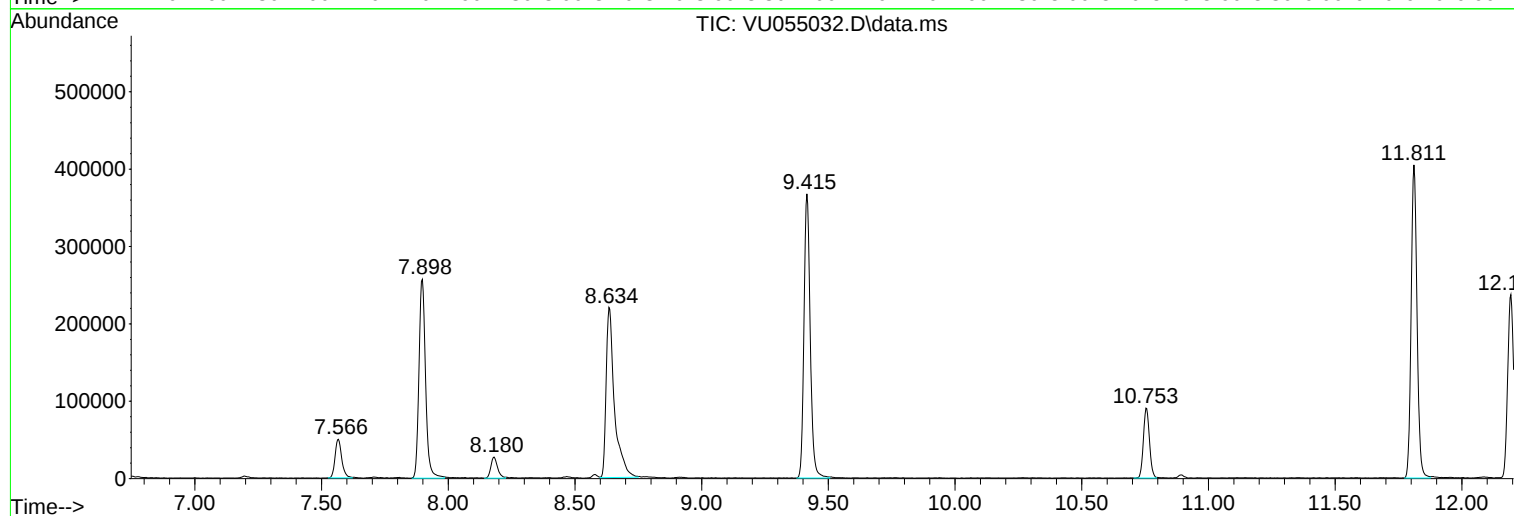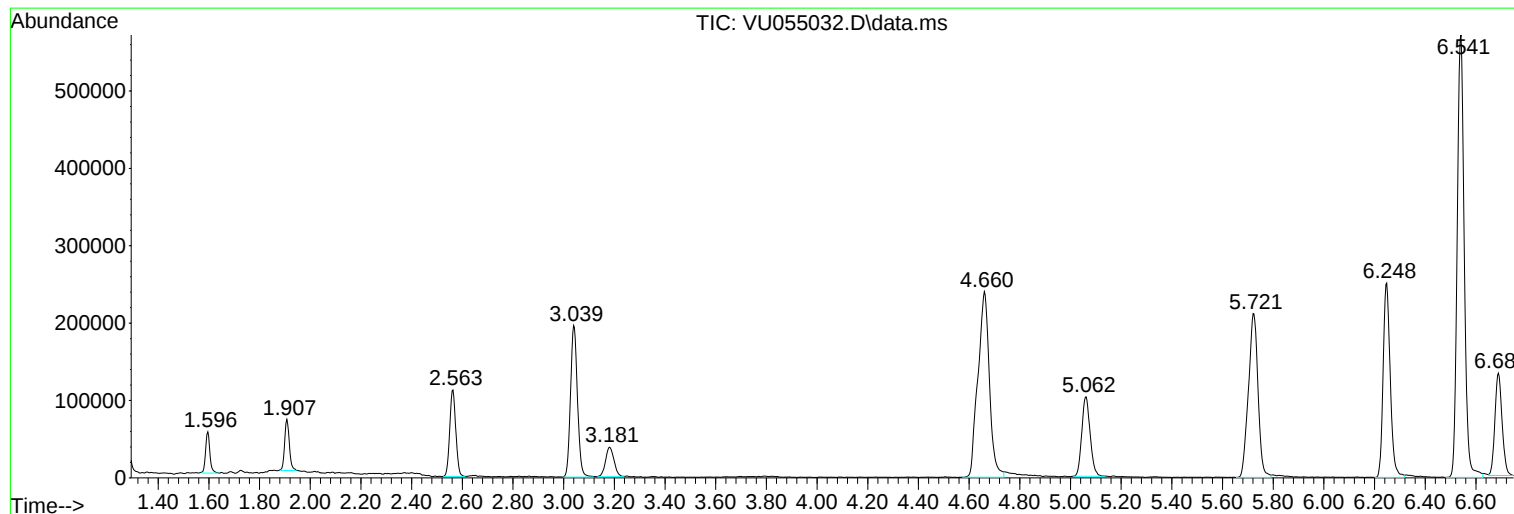

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055032.D
Acq On : 31 Aug 2023 19:42
Operator : MD/SY
Sample : 04153-06 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH464

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055032.D
Acq On : 31 Aug 2023 19:42
Operator : MD/SY
Sample : 04153-06 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH464

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------