
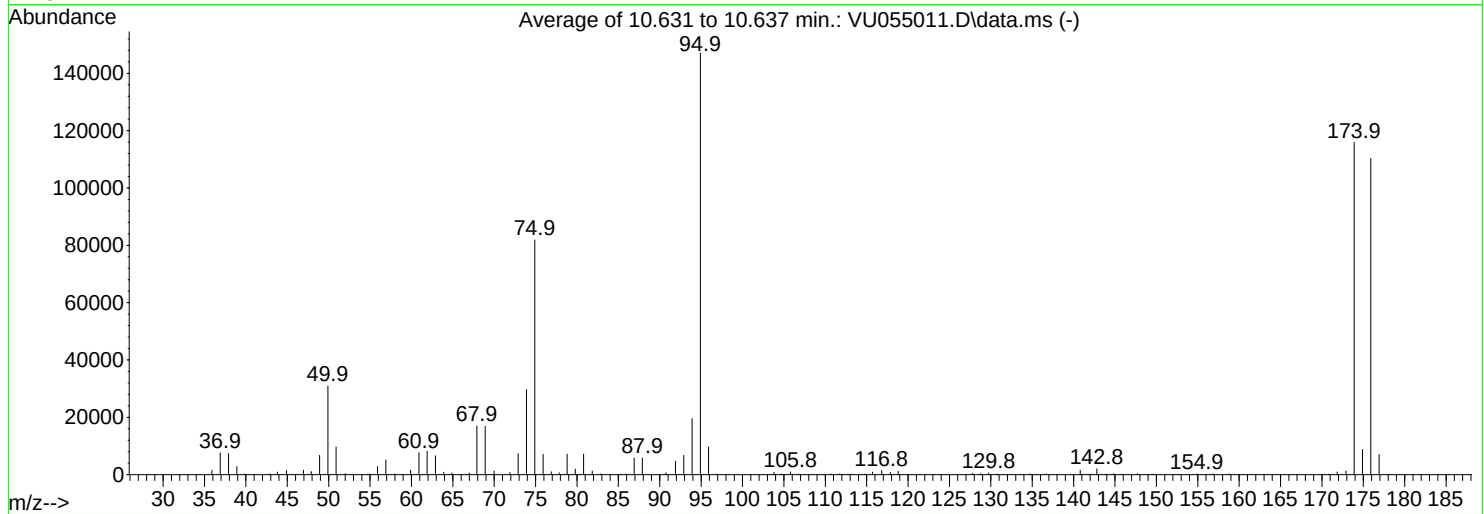


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083123\
Data File : VU055011.D
Acq On : 31 Aug 2023 08:36
Operator : MD/SY
Sample : BFB037
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB037

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 01 04:57:47 2023

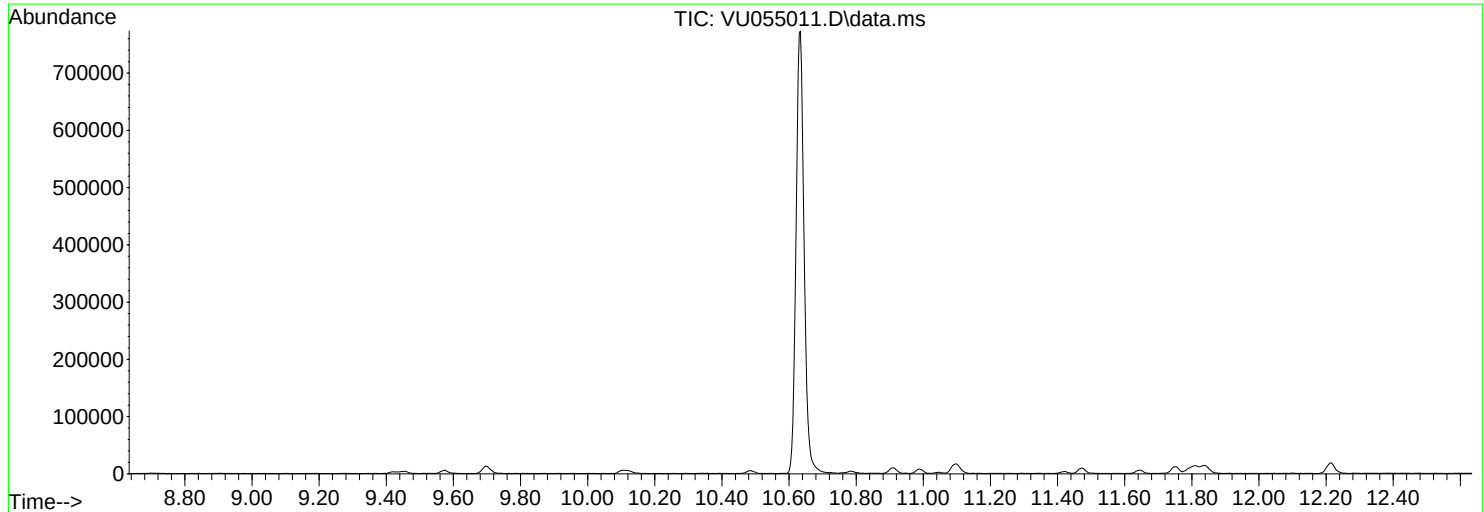

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	30923	PASS
75	95	30	80	55.6	81800	PASS
95	95	100	100	100.0	147136	PASS
96	95	5	9	6.6	9645	PASS
173	174	0.00	2	1.1	1267	PASS
174	95	50	120	78.8	115907	PASS
175	174	5	9	7.6	8795	PASS
176	174	95	101	95.2	110339	PASS
177	176	5	9	6.4	7053	PASS

m/z	Abundance
39.80	146.0
43.90	842.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	1487.0
36.90	8002.0
37.90	7625.0
38.90	3031.0
39.80	415.0
42.90	277.0
43.80	1629.0
44.90	1517.0
47.00	1727.0
47.90	1135.0
48.90	7166.0
49.90	32216.0
50.90	10004.0
52.00	352.0
52.90	118.0
54.70	428.0
55.90	2913.0
56.90	5211.0
57.90	295.0
59.90	1619.0
60.90	7970.0
61.90	8238.0
62.90	6782.0
63.90	702.0
64.90	573.0
67.00	569.0
67.90	17936.0
68.90	17752.0
70.00	1445.0
71.90	895.0
72.90	7432.0
73.90	30840.0
74.90	86224.0
75.90	7525.0
76.90	1022.0
77.80	553.0
78.80	7667.0
79.80	2009.0
80.80	7318.0
81.90	1311.0
82.90	263.0
85.90	241.0
86.90	5805.0
87.90	6130.0
90.80	638.0
91.90	5070.0
92.90	7200.0
93.90	20512.0
94.90	150528.0
95.90	10069.0
96.90	256.0
103.80	886.0
104.80	204.0
105.80	868.0
106.70	216.0
109.80	175.0
110.70	295.0
111.80	218.0
112.80	249.0
114.70	204.0
115.70	844.0
116.80	1354.0
117.90	764.0
118.80	1113.0
125.80	103.0
127.80	482.0
128.70	364.0
129.80	530.0
130.80	193.0
134.70	312.0
136.80	266.0
140.80	1546.0
141.80	249.0
142.80	1982.0
143.90	124.0
144.90	263.0
145.90	147.0
147.70	364.0
148.90	166.0
149.80	203.0
152.70	133.0
154.90	331.0
156.80	328.0
158.80	263.0
170.80	184.0
171.90	950.0
172.90	1347.0
173.90	116656.0
174.90	9076.0
175.90	109640.0
176.90	6930.0
177.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

178.10

125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	1521.0
36.90	7846.0
37.90	7585.0
38.90	2890.0
39.90	388.0
42.90	274.0
43.80	1728.0
44.90	1472.0
45.80	123.0
47.00	1573.0
47.90	1082.0
48.90	6878.0
49.90	31984.0
50.90	9806.0
52.10	318.0
52.90	169.0
54.90	454.0
55.90	2940.0
56.90	5231.0
57.90	277.0
59.90	1603.0
60.90	7864.0
61.90	8321.0
62.90	6850.0
63.90	909.0
64.90	579.0
67.00	587.0
67.90	17752.0
68.90	17160.0
70.00	1362.0
71.90	808.0
72.90	7449.0
73.90	30488.0
74.90	83968.0
75.90	7239.0
76.90	1001.0
77.90	669.0
78.80	7504.0
79.80	1963.0
80.80	7413.0
81.80	1328.0
82.90	232.0
85.90	336.0
86.90	5998.0
87.90	5943.0
90.70	666.0
91.90	4840.0
92.90	6838.0
93.90	20192.0
94.90	151296.0
95.90	9885.0
96.90	256.0
103.80	871.0
104.70	231.0
105.80	946.0
106.70	186.0
109.80	164.0
110.70	237.0
111.10	127.0
111.80	258.0
112.70	184.0
114.80	202.0
115.70	923.0
116.80	1551.0
117.80	802.0
118.80	1245.0
125.80	106.0
127.80	521.0
128.80	339.0
129.70	549.0
130.70	233.0
134.70	284.0
136.70	238.0
139.60	104.0
140.00	116.0
140.80	1569.0
141.80	183.0
142.80	2038.0
143.90	162.0
144.80	348.0
145.90	181.0
147.70	372.0
148.90	159.0
149.60	183.0
152.70	120.0
154.90	310.0
156.90	307.0
158.70	237.0
170.40	120.0
170.80	157.0
171.80	1036.0
172.90	1322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

173.90	119960.0
174.90	9165.0
175.90	113968.0
176.90	7277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	1457.0
36.90	6960.0
37.90	6878.0
38.90	2483.0
39.90	301.0
42.90	225.0
43.80	1795.0
44.90	1337.0
45.80	173.0
46.90	1344.0
47.90	976.0
48.90	6149.0
49.90	28568.0
50.90	9091.0
52.10	285.0
52.90	141.0
54.90	456.0
55.90	2641.0
56.90	4939.0
58.00	224.0
59.90	1466.0
60.90	7075.0
61.90	7835.0
62.90	6213.0
63.90	974.0
64.90	632.0
67.00	551.0
67.90	15277.0
68.90	15592.0
70.00	1115.0
71.90	733.0
72.90	7062.0
73.90	27576.0
74.90	75208.0
75.90	6436.0
76.90	984.0
77.90	623.0
78.80	6476.0
79.80	1865.0
80.80	6664.0
81.80	1225.0
82.80	176.0
85.90	356.0
86.90	5555.0
87.90	5319.0
90.70	711.0
91.90	4201.0
92.90	6306.0
93.90	18056.0
94.90	139584.0
95.90	8981.0
96.90	201.0
103.80	851.0
104.70	248.0
105.80	1012.0
106.80	139.0
109.90	202.0
110.70	139.0
111.10	101.0
111.70	258.0
112.80	145.0
114.90	207.0
115.70	855.0
116.80	1423.0
117.80	719.0
118.80	1207.0
127.80	524.0
128.90	263.0
129.70	551.0
130.70	262.0
134.70	246.0
136.60	260.0
139.60	110.0
139.90	100.0
140.80	1535.0
141.70	154.0
142.80	1985.0
143.80	199.0
144.80	331.0
145.90	204.0
147.70	323.0
149.60	190.0
154.90	265.0
156.90	225.0
158.90	204.0
170.30	104.0
170.90	100.0
171.80	912.0
172.90	1131.0
173.90	111104.0
174.90	8145.0
175.90	107408.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

176.90

6951.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037