


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090119\
 Data File : VU034113.D
 Acq On : 31 Aug 2019 08:45
 Operator : JC/SP
 Sample : BFB06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR090119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sun Sep 01 01:40:37 2019

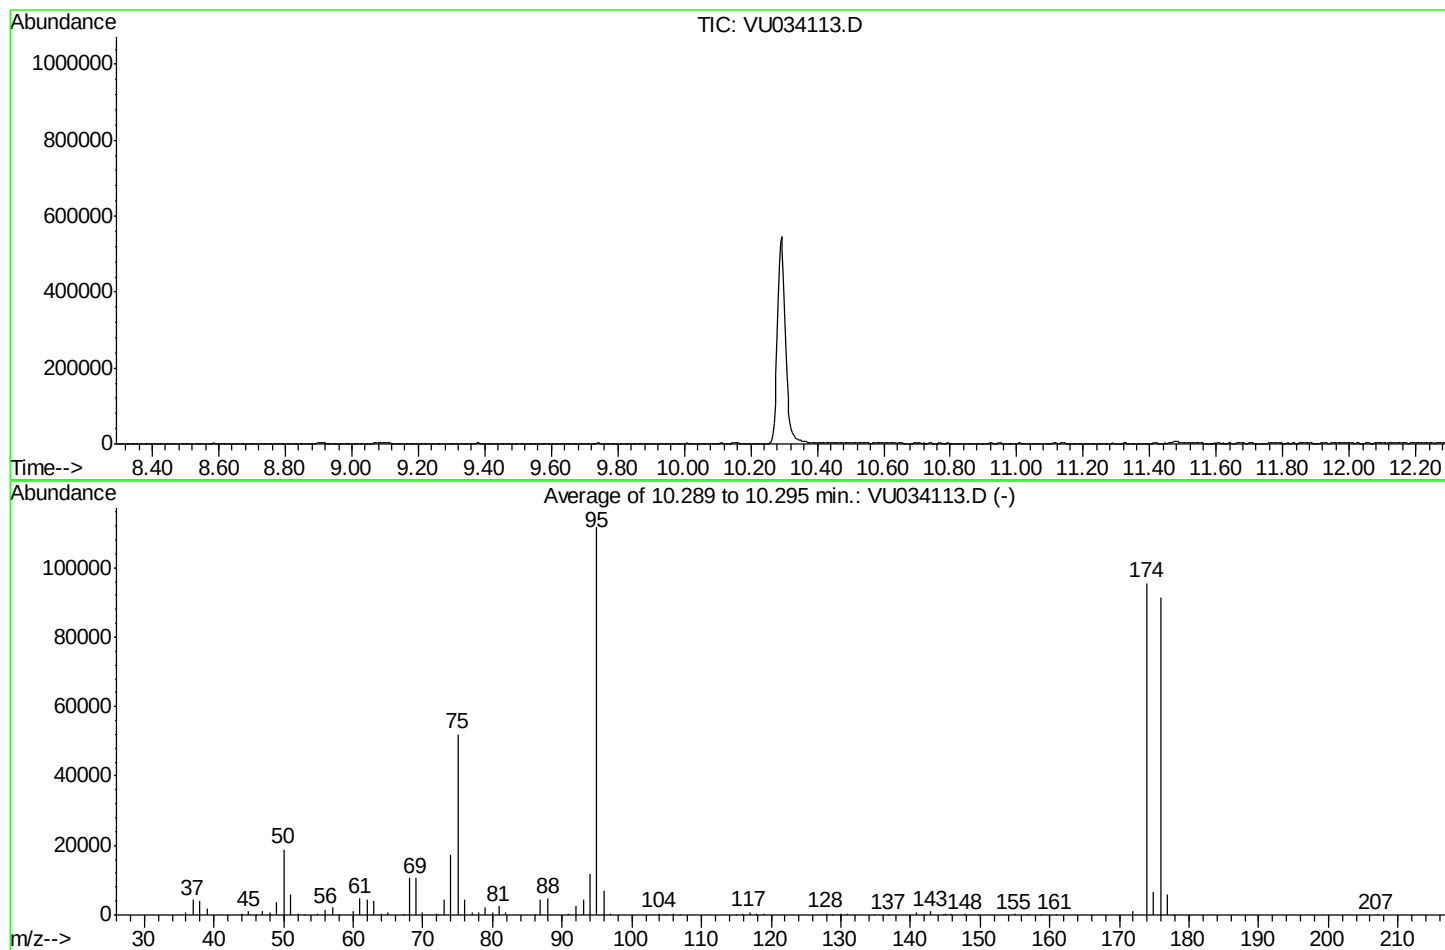

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	18866	PASS
75	95	30	80	46.7	52085	PASS
95	95	100	100	100.0	111613	PASS
96	95	5	9	6.2	6954	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	95541	PASS
175	174	5	9	6.9	6620	PASS
176	174	95	101	95.6	91349	PASS
177	176	5	9	6.5	5923	PASS

m/z	Abundance
36.00	1062.0
37.00	4324.0
38.00	4173.0
39.00	2055.0
40.00	418.0
42.90	106.0
43.90	1120.0
45.00	863.0
46.10	106.0
47.00	1080.0
48.00	630.0
49.00	3672.0
50.00	20072.0
51.00	5899.0
52.00	338.0
54.90	350.0
56.00	1512.0
57.00	2363.0
58.00	158.0
60.00	934.0
61.00	4828.0
62.00	4754.0
63.00	4091.0
64.00	600.0
65.00	761.0
67.10	222.0
68.00	10610.0
69.00	10924.0
70.00	825.0
71.90	601.0
73.00	4306.0
74.00	17760.0
75.00	53600.0
76.00	4624.0
77.00	684.0
78.00	583.0
78.90	2386.0
80.00	712.0
80.90	2602.0
81.90	576.0
86.10	123.0
86.90	4684.0
87.90	4820.0
91.00	364.0
92.00	2908.0
93.00	4722.0
94.00	12026.0
95.00	112304.0
96.00	6935.0
97.00	263.0
104.00	417.0
104.80	138.0
105.90	360.0
106.90	163.0
115.00	119.0
115.90	299.0
117.00	706.0
117.90	339.0
118.90	463.0
128.00	383.0
128.80	140.0
129.90	391.0
130.90	245.0
134.70	180.0
136.90	150.0
140.90	814.0
141.90	111.0
142.90	1187.0
144.80	165.0
145.20	203.0
145.90	226.0
147.90	258.0
149.70	119.0
155.00	282.0
156.90	180.0
160.80	100.0
171.90	1072.0
174.00	95032.0
174.90	6791.0
176.00	89592.0
176.90	6078.0
207.00	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	949.0
37.00	4415.0
38.00	4196.0
39.00	1981.0
40.00	385.0
42.90	145.0
43.90	1089.0
45.00	984.0
46.10	125.0
47.00	1052.0
48.00	604.0
49.00	3665.0
50.00	19384.0
51.10	5979.0
52.00	290.0
53.00	101.0
54.90	276.0
56.00	1558.0
57.00	2306.0
58.00	135.0
60.00	1013.0
61.00	4956.0
62.00	4706.0
63.00	4089.0
64.00	542.0
65.00	736.0
67.10	249.0
68.00	10818.0
69.00	11001.0
70.00	841.0
71.90	563.0
73.00	4468.0
74.00	17848.0
75.00	53656.0
76.10	4615.0
77.00	670.0
78.00	610.0
78.90	2466.0
80.00	792.0
80.90	2508.0
81.90	628.0
86.00	146.0
86.90	4781.0
88.00	4807.0
90.90	342.0
92.00	2809.0
93.00	4655.0
94.00	12060.0
95.00	115216.0
96.00	7183.0
97.00	283.0
104.00	495.0
104.80	122.0
105.90	348.0
106.90	173.0
114.90	105.0
115.90	289.0
116.90	800.0
117.90	383.0
118.90	520.0
128.00	454.0
128.80	176.0
130.00	408.0
130.90	268.0
134.80	148.0
136.90	164.0
140.90	860.0
142.90	1156.0
145.20	221.0
145.90	235.0
147.90	311.0
149.80	122.0
154.90	290.0
156.90	169.0
160.80	122.0
171.90	1109.0
174.00	98592.0
174.90	6816.0
176.00	94424.0
177.00	6143.0
177.90	115.0
207.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	755.0
37.00	4235.0
38.00	3921.0
39.10	1678.0
39.90	403.0
42.90	166.0
44.00	1172.0
45.00	1039.0
46.10	131.0
47.00	983.0
48.00	525.0
49.00	3535.0
50.00	17144.0
51.10	5579.0
52.00	234.0
54.90	196.0
56.00	1376.0
57.00	2176.0
60.00	1029.0
61.00	4560.0
62.10	4375.0
63.00	3669.0
64.00	441.0
65.00	682.0
68.00	10120.0
69.00	9928.0
70.00	786.0
72.10	458.0
73.00	4243.0
74.00	16256.0
75.00	49000.0
76.10	4161.0
77.00	629.0
77.90	585.0
78.90	2365.0
79.90	763.0
80.90	2244.0
81.90	626.0
86.00	160.0
86.90	4344.0
88.00	4247.0
90.90	300.0
92.00	2518.0
93.00	4222.0
94.00	11364.0
95.00	107320.0
96.10	6745.0
97.00	235.0
104.00	570.0
105.90	359.0
106.90	144.0
115.80	272.0
116.90	758.0
117.90	388.0
118.90	559.0
127.90	465.0
128.70	185.0
129.90	384.0
130.90	246.0
134.90	113.0
136.90	161.0
140.90	891.0
142.90	938.0
145.00	209.0
145.90	197.0
147.90	296.0
149.80	119.0
154.90	296.0
156.90	131.0
158.70	104.0
171.90	1136.0
174.00	93000.0
174.90	6253.0
176.00	90032.0
177.00	5550.0
177.80	151.0
206.90	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

Scan 2848 (10.247 min): VU034113.D
BFB06

m/z	Abundance
40.00	484.0
43.00	152.0
44.00	784.0
63.80	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06