


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090120\
Data File : VU040008.D
Acq On : 01 Sep 2020 10:20
Operator : SY/MD
Sample : BFB25
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Sep 01 17:18:02 2020

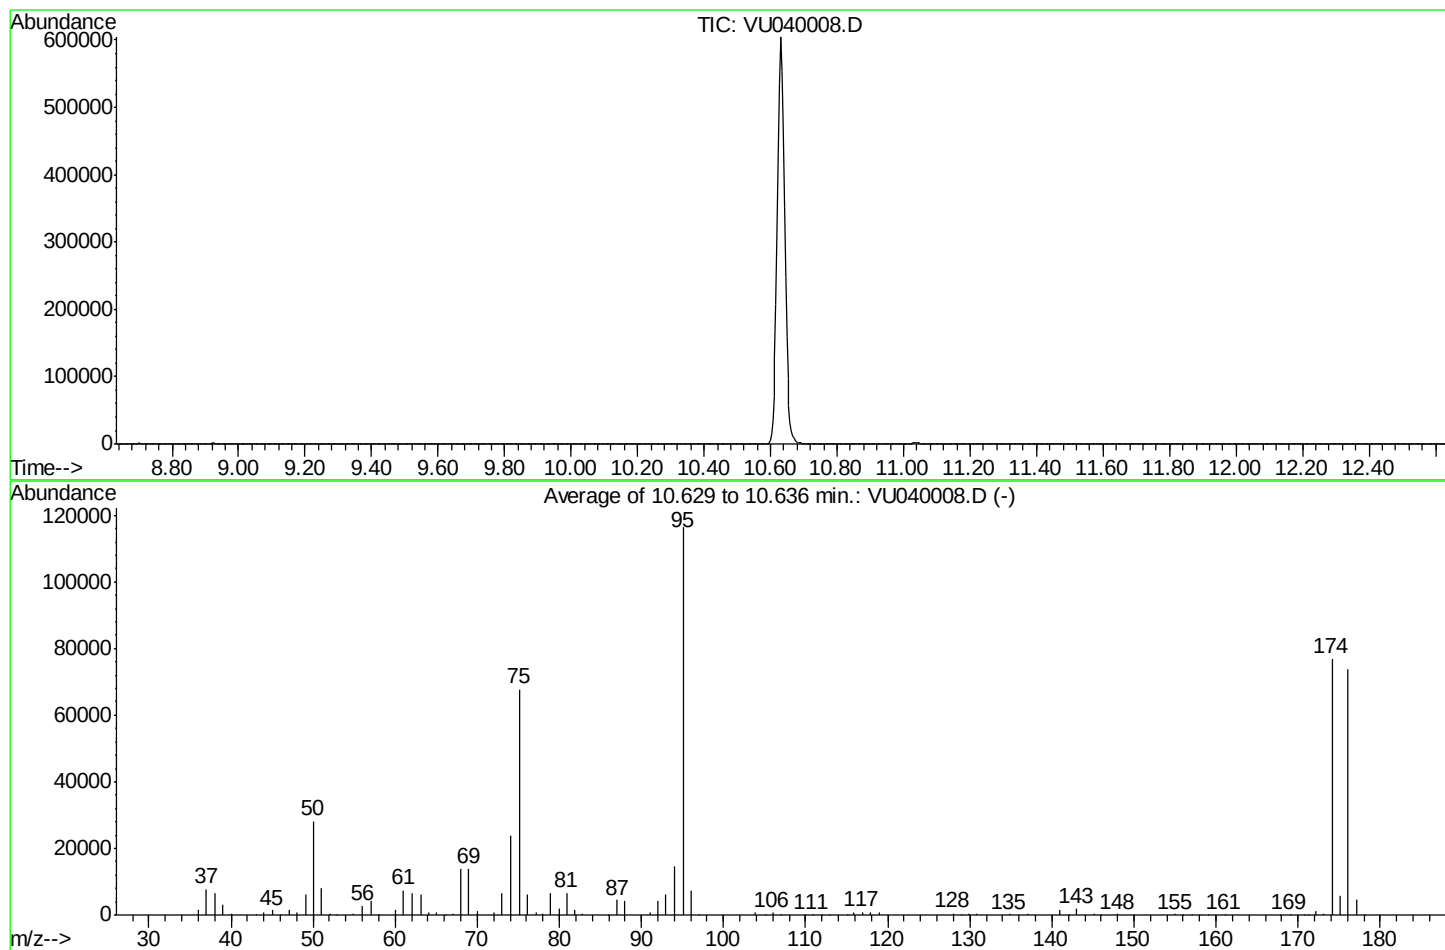

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	28157	PASS
75	95	30	80	58.2	67738	PASS
95	95	100	100	100.0	116389	PASS
96	95	5	9	6.4	7467	PASS
173	174	0.00	2	0.6	429	PASS
174	95	50	120	66.2	77029	PASS
175	174	5	9	7.6	5835	PASS
176	174	95	101	95.6	73616	PASS
177	176	5	9	6.4	4701	PASS

m/z	Abundance
36.00	1395.0
37.00	8416.0
38.00	7236.0
39.10	3016.0
40.00	233.0
44.00	1281.0
45.00	1476.0
45.90	238.0
47.00	1571.0
48.00	925.0
49.00	6528.0
50.00	29432.0
51.00	8368.0
52.10	315.0
52.90	138.0
54.90	548.0
56.00	3100.0
57.00	4637.0
57.90	142.0
60.00	1462.0
61.00	7771.0
62.10	7199.0
63.10	6041.0
64.10	900.0
65.00	820.0
66.10	147.0
67.00	492.0
68.00	14015.0
69.00	13994.0
70.00	1089.0
72.10	807.0
73.10	6699.0
74.00	23896.0
75.10	70080.0
76.10	6478.0
77.10	870.0
77.90	494.0
78.90	6973.0
80.00	2004.0
80.90	6697.0
81.90	1552.0
82.80	294.0
85.90	135.0
87.00	4615.0
88.00	4209.0
91.00	675.0
92.00	4434.0
93.00	6367.0
94.10	15057.0
95.10	119248.0
96.10	7737.0
97.00	256.0
103.90	607.0
105.00	191.0
106.00	689.0
106.90	163.0
109.90	129.0
110.90	178.0
111.90	189.0
113.00	138.0
115.00	117.0
115.80	618.0
116.90	953.0
118.00	653.0
119.00	790.0
128.00	613.0
129.10	164.0
130.00	448.0
130.90	217.0
134.80	213.0
137.00	261.0
141.00	1624.0
142.10	176.0
143.00	1671.0
145.10	291.0
145.90	185.0
148.10	261.0
150.00	148.0
155.00	236.0
157.00	159.0
159.00	184.0
161.00	195.0
167.80	135.0
168.90	125.0
170.80	203.0
172.10	1273.0
173.10	1289.0
174.10	76488.0
175.10	5879.0
176.10	73472.0
177.10	4747.0
178.00	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	1485.0
37.00	7990.0
38.00	6767.0
39.00	3065.0
40.00	246.0
43.00	133.0
44.00	1332.0
45.00	1414.0
46.00	183.0
47.10	1777.0
48.10	871.0
49.10	6417.0
50.00	29136.0
51.00	8176.0
52.10	339.0
52.90	110.0
54.90	498.0
56.00	2922.0
57.00	4580.0
58.00	174.0
60.00	1409.0
61.00	7698.0
62.00	6769.0
63.10	6207.0
64.10	733.0
65.00	834.0
66.10	174.0
67.00	491.0
68.00	14146.0
69.00	14522.0
70.00	1137.0
72.10	916.0
73.00	6659.0
74.00	24528.0
75.10	69968.0
76.10	6500.0
77.10	768.0
77.90	573.0
78.90	6746.0
79.90	1968.0
80.90	6847.0
81.90	1550.0
82.80	242.0
85.80	130.0
87.10	4693.0
88.00	4595.0
91.00	743.0
92.00	4421.0
93.00	6208.0
94.10	14715.0
95.10	120152.0
96.10	7657.0
97.00	220.0
103.90	674.0
105.00	162.0
106.00	679.0
107.00	163.0
109.90	153.0
110.80	170.0
111.90	180.0
113.00	156.0
115.00	129.0
115.90	656.0
116.90	1037.0
118.00	705.0
119.00	783.0
128.00	483.0
129.00	182.0
129.90	462.0
130.90	250.0
134.80	268.0
137.00	232.0
141.00	1676.0
142.00	177.0
143.00	1848.0
145.10	280.0
145.90	191.0
148.10	298.0
150.00	158.0
155.00	309.0
155.90	109.0
157.00	192.0
157.90	105.0
159.00	210.0
161.00	180.0
169.00	100.0
170.80	148.0
171.20	139.0
172.20	1306.0
174.10	79704.0
175.10	6099.0
176.10	76280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

177.104863.0

178.10162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	1357.0
37.00	6991.0
38.00	5935.0
39.00	2814.0
40.00	265.0
43.00	153.0
44.00	1246.0
45.00	1314.0
46.10	163.0
47.00	1681.0
48.10	751.0
49.10	5762.0
50.00	25904.0
51.00	7201.0
52.00	305.0
55.00	391.0
56.00	2464.0
57.00	4044.0
58.00	190.0
60.00	1297.0
61.00	6948.0
62.00	6239.0
63.10	5687.0
64.00	657.0
65.10	762.0
66.10	137.0
67.00	421.0
68.00	12887.0
69.00	13261.0
70.00	988.0
72.10	886.0
73.10	5980.0
74.00	22656.0
75.10	63168.0
76.00	5908.0
77.20	613.0
77.90	548.0
78.90	6054.0
79.90	1715.0
80.90	6429.0
81.90	1442.0
82.90	116.0
85.80	133.0
87.10	4229.0
88.00	4383.0
91.00	716.0
92.00	3950.0
93.00	5593.0
94.10	13629.0
95.10	109768.0
96.10	7007.0
97.00	145.0
103.90	677.0
105.10	140.0
106.00	612.0
107.00	165.0
109.90	137.0
110.80	132.0
111.90	110.0
112.90	162.0
115.00	101.0
115.90	586.0
117.00	899.0
117.90	594.0
119.00	676.0
128.00	331.0
128.90	175.0
129.90	437.0
130.90	253.0
134.80	299.0
137.00	164.0
141.00	1505.0
142.00	193.0
143.00	1841.0
145.10	222.0
145.90	162.0
148.00	312.0
150.00	136.0
155.00	284.0
155.90	108.0
157.00	223.0
159.10	195.0
161.00	150.0
171.20	152.0
172.20	1177.0
174.10	74896.0
175.10	5528.0
176.10	71096.0
177.10	4494.0
178.10	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
44.00	317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25