

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
 Data File : VU044543.D
 Acq On : 01 Sep 2021 10:27
 Operator : SY/MD
 Sample : VU0901WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0901WBL01

Quant Time: Sep 02 11:43:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Sep 01 01:29:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	19492	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	5993	0.803	ug/l	0.00
Spiked Amount 1.000			Recovery	=	80.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	10405	1.202	ug/l	0.00
Spiked Amount 1.000			Recovery	=	120.000%	
Target Compounds						
15) Methylene Chloride	3.054	84	7609	0.528	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044543.D
Acq On : 01 Sep 2021 10:27
Operator : SY/MD
Sample : VU0901WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01

Quant Time: Sep 02 11:43:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Sep 01 01:29:46 2021
Response via : Initial Calibration




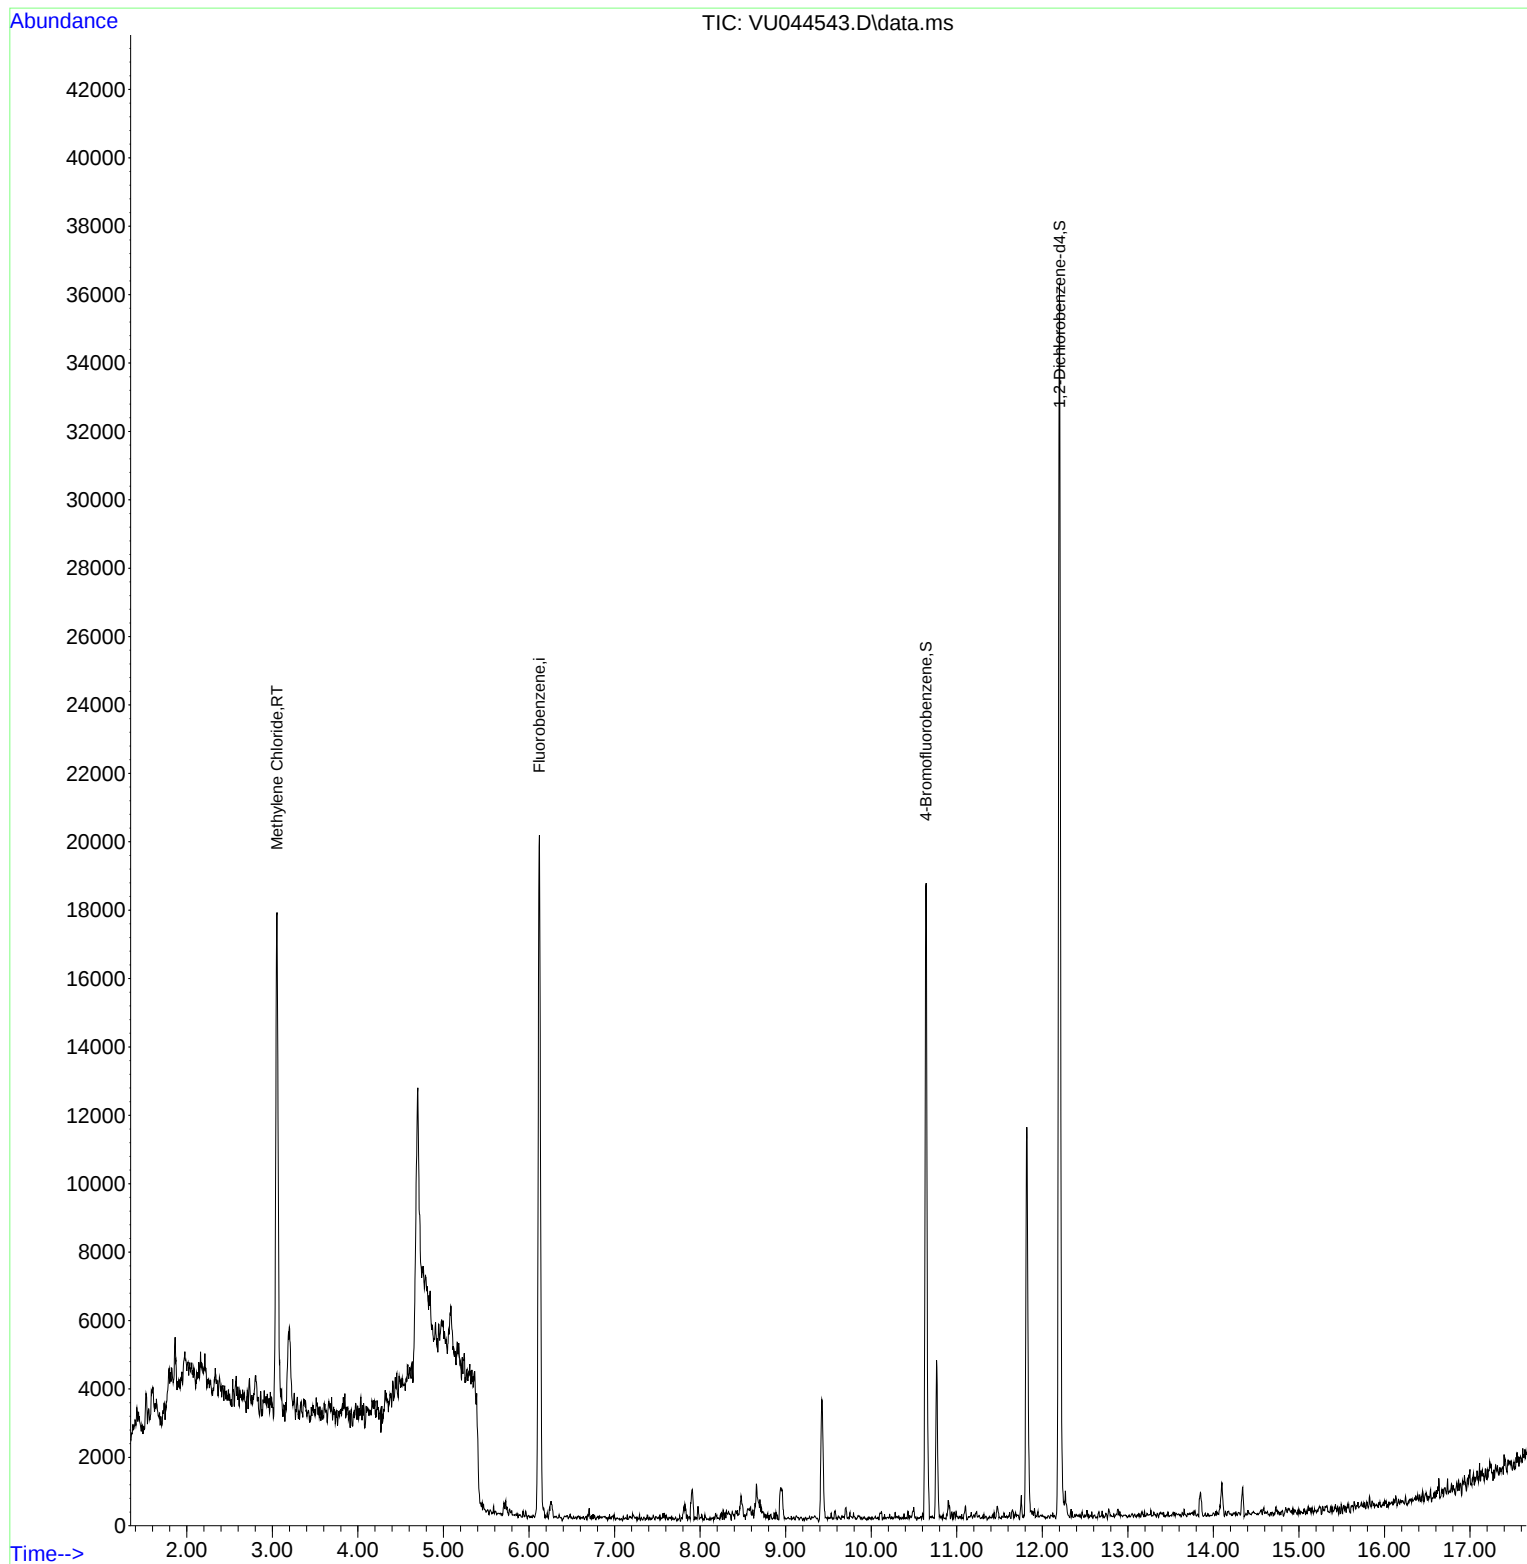


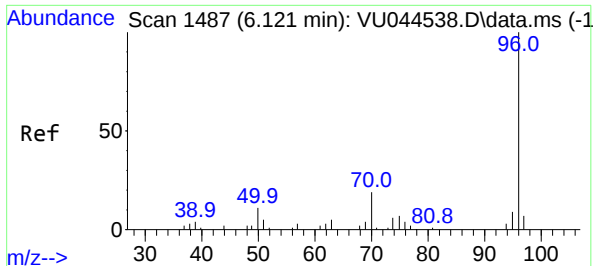

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU044543.D
Acq: 01 Sep 2021 10:27




Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01


Tgt Ion:	96	Resp:	19492
Ion	Ratio	Lower	Upper
96	100		
70	18.1	16.2	24.2
95	9.2	7.0	10.6
97	6.0	0.0	0.0

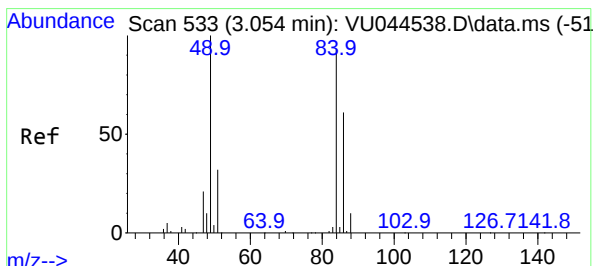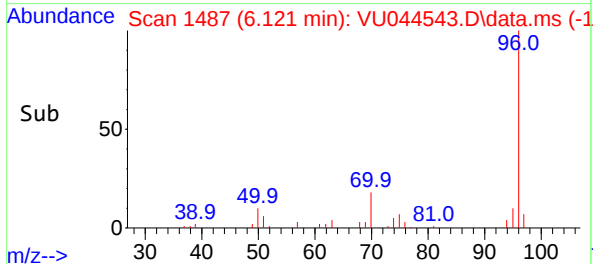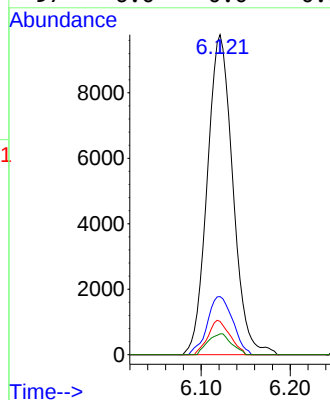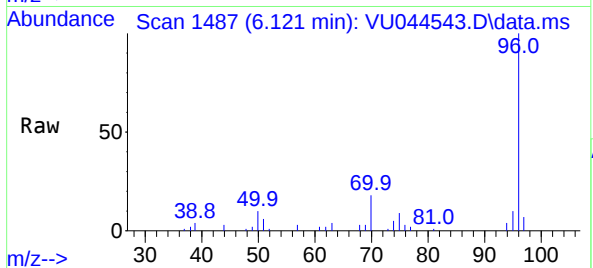

#15
Methylene Chloride
Concen: 0.528 ug/l
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU044543.D
Acq: 01 Sep 2021 10:27

Tgt Ion:	84	Resp:	7609
Ion	Ratio	Lower	Upper
84	100		
49	97.6	85.6	128.4
51	32.4	0.0	67.6
86	60.6	52.1	78.1


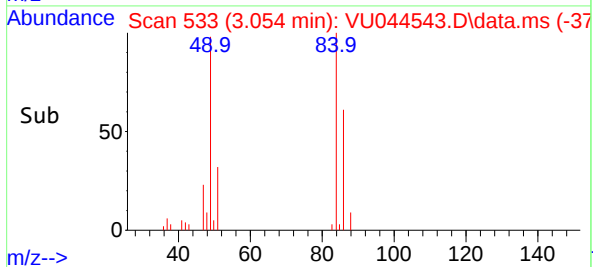
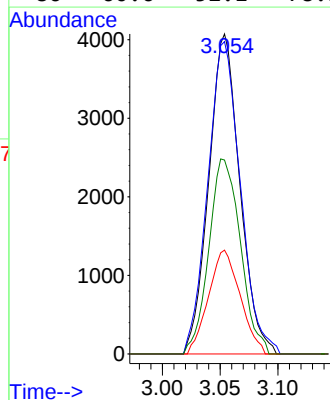
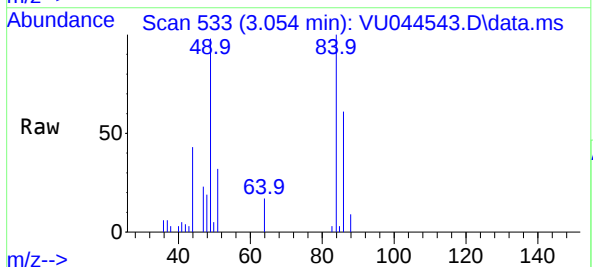


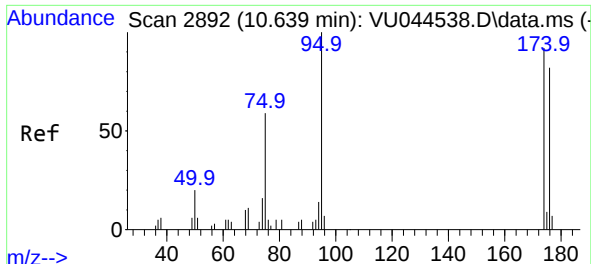

#57
4-Bromofluorobenzene
Concen: 0.803 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU044543.D
Acq: 01 Sep 2021 10:27

Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01

Tgt Ion:	95	Resp:	5993
Ion	Ratio	Lower	Upper
95	100		
174	92.7	65.9	98.9
176	92.0	63.0	94.4

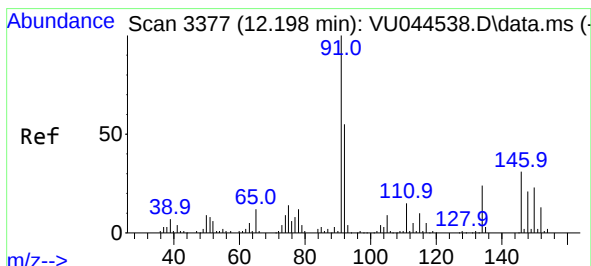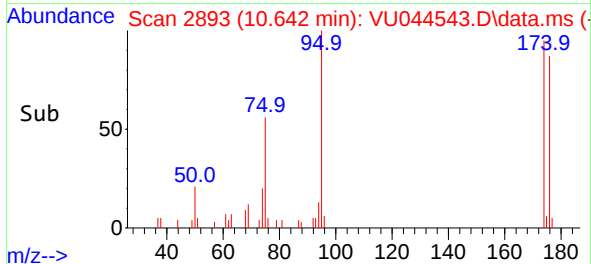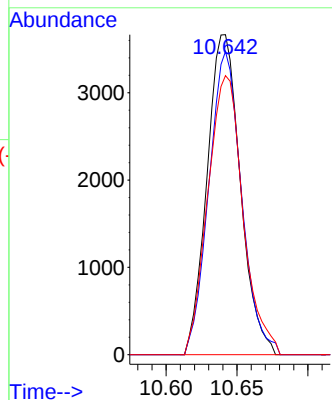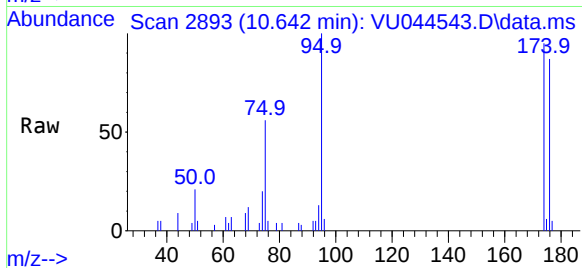

#68
1,2-Dichlorobenzene-d4
Concen: 1.202 ug/l
RT: 12.201 min Scan# 3378
Delta R.T. 0.003 min
Lab File: VU044543.D
Acq: 01 Sep 2021 10:27

Tgt Ion:	152	Resp:	10405
Ion	Ratio	Lower	Upper
152	100		
115	59.5	0.0	277.8
150	155.5	0.0	674.2

