

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
 Data File : VU044545.D
 Acq On : 01 Sep 2021 12:31
 Operator : SY/MD
 Sample : M3604-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-083021

Quant Time: Sep 02 11:43:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Sep 01 01:29:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	18844	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	6000	0.832	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	6824	0.815	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	
Target Compounds						
15) Methylene Chloride	3.054	84	6937	0.498	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044545.D
Acq On : 01 Sep 2021 12:31
Operator : SY/MD
Sample : M3604-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Quant Time: Sep 02 11:43:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Sep 01 01:29:46 2021
Response via : Initial Calibration

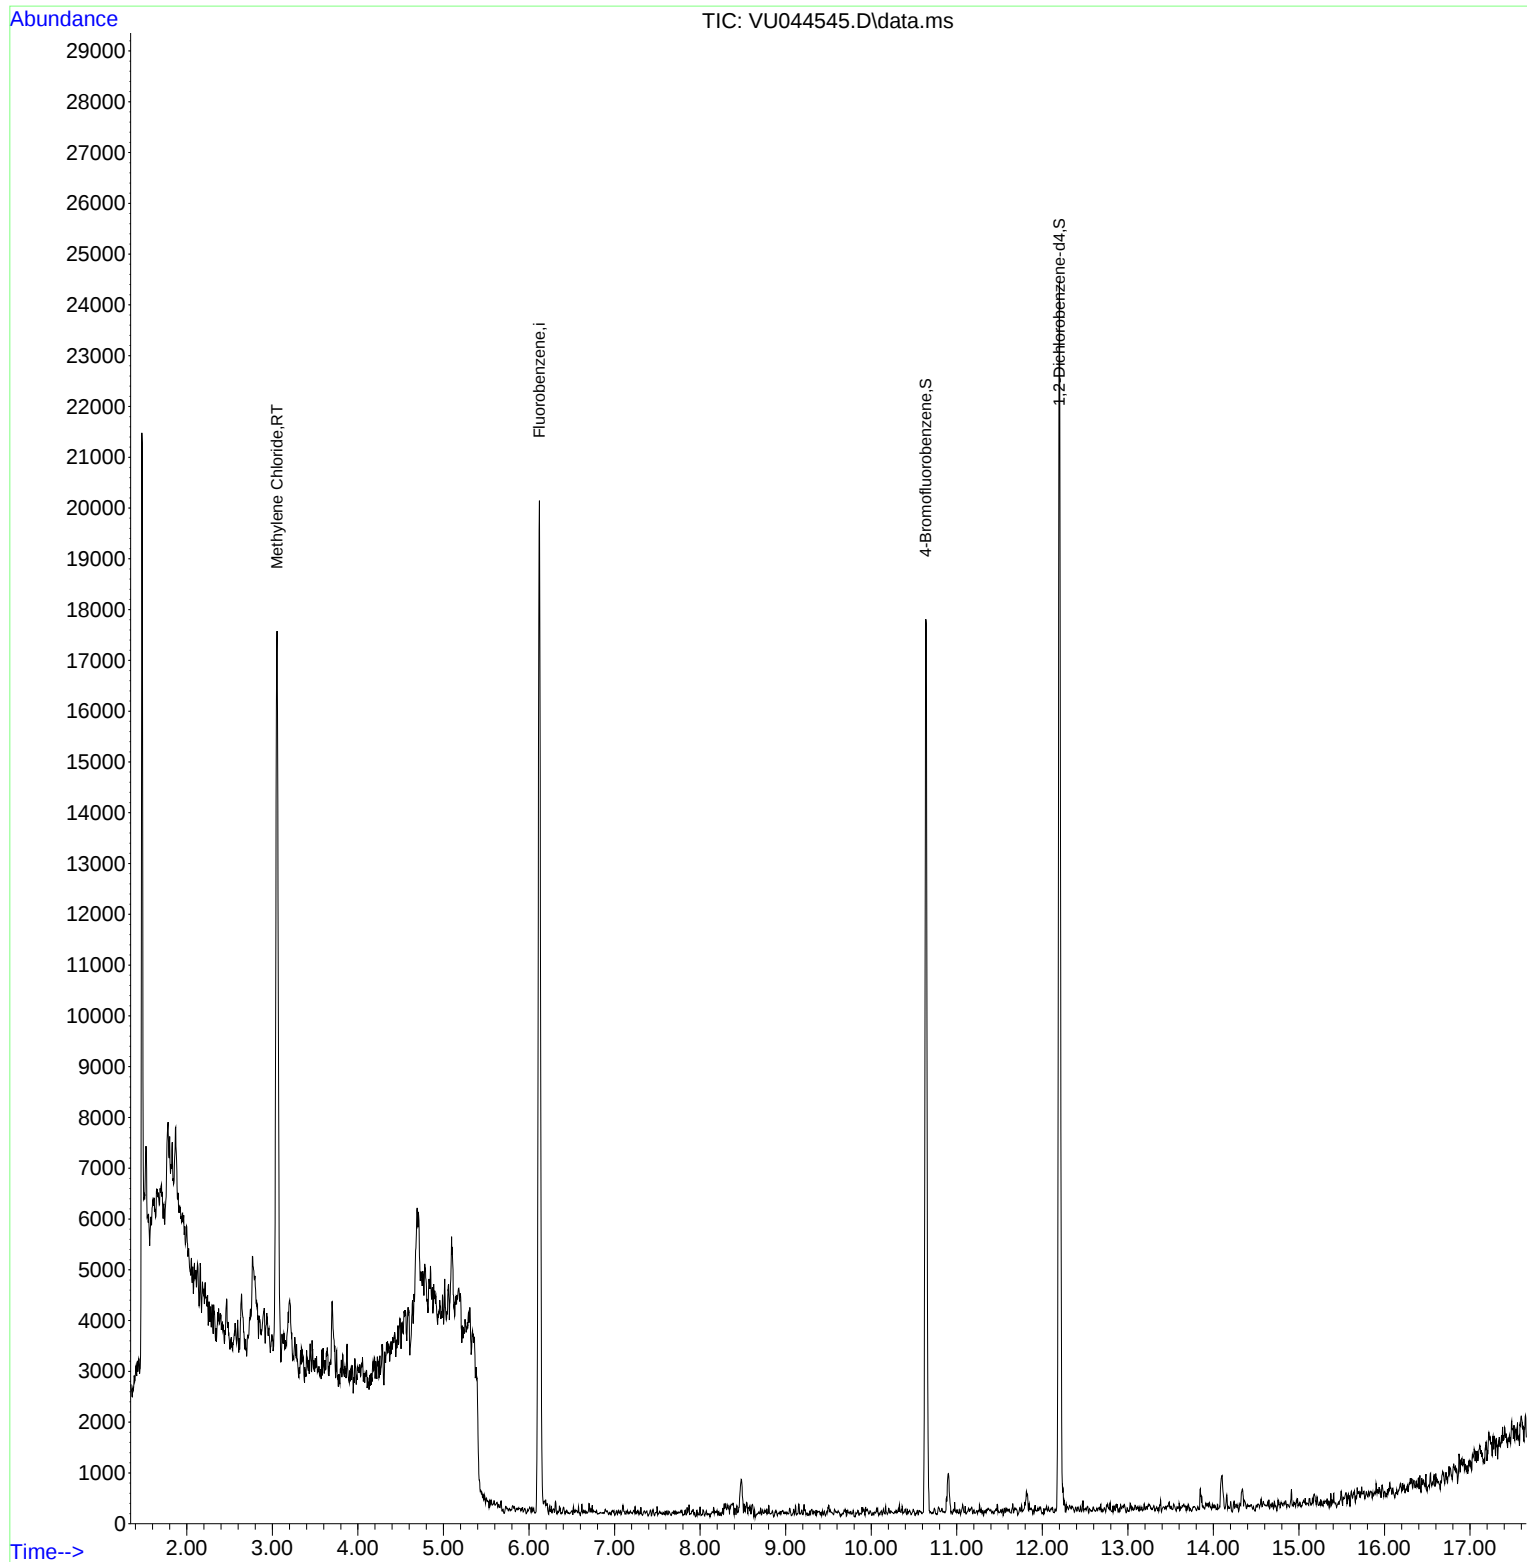




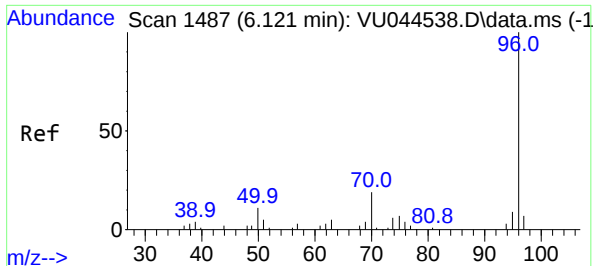


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU044545.D
Acq: 01 Sep 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Tgt Ion: 96 Resp: 18844




Ion	Ratio	Lower	Upper
96	100		
70	16.9	16.2	24.2
95	8.6	7.0	10.6
97	6.6	0.0	0.0

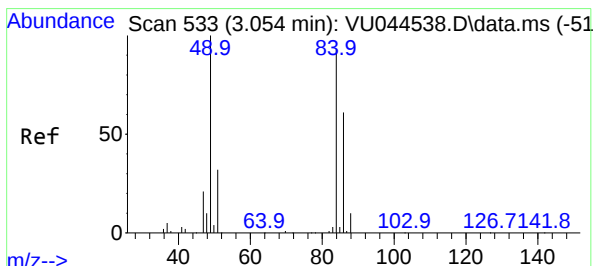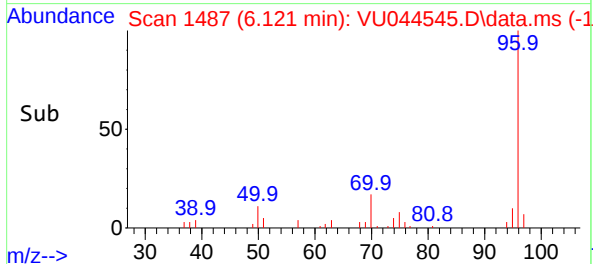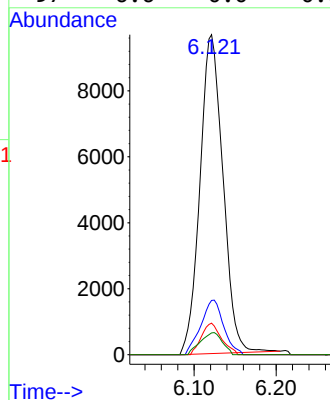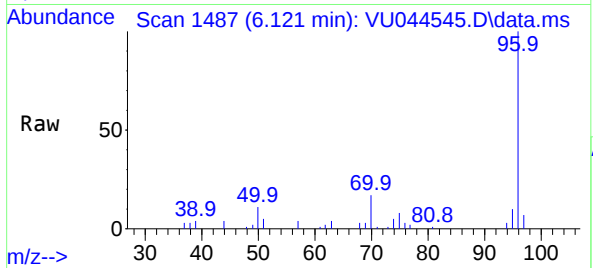


#15
Methylene Chloride
Concen: 0.498 ug/l
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU044545.D
Acq: 01 Sep 2021 12:31

Tgt Ion: 84 Resp: 6937

Ion	Ratio	Lower	Upper
84	100		
49	118.8	85.6	128.4
51	41.3	0.0	67.6
86	70.9	52.1	78.1


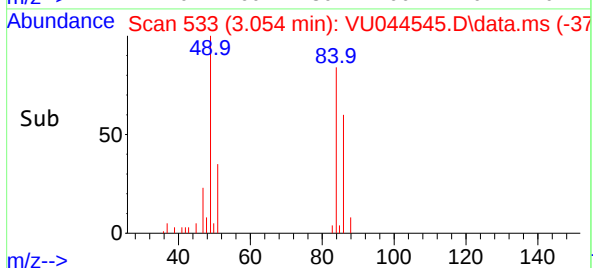
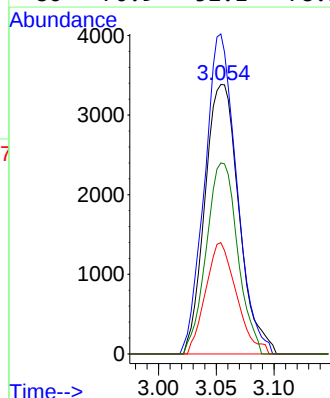
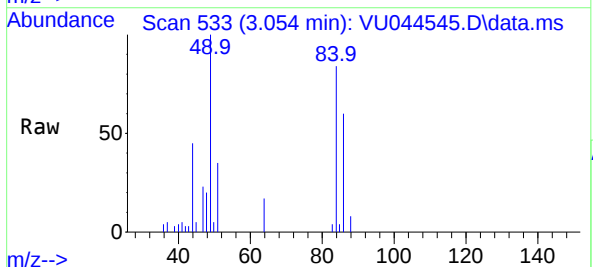


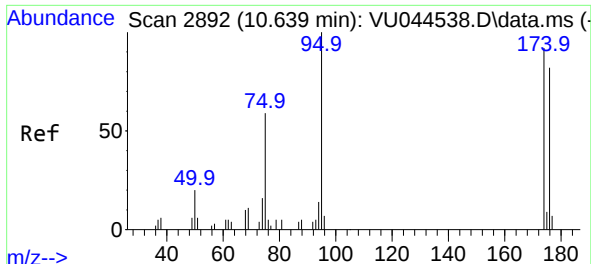

#57
4-Bromofluorobenzene
Concen: 0.832 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044545.D
Acq: 01 Sep 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Tgt Ion: 95 Resp: 6000
Ion Ratio Lower Upper
95 100
174 89.9 65.9 98.9
176 83.5 63.0 94.4

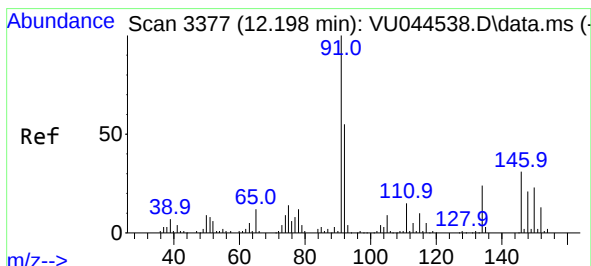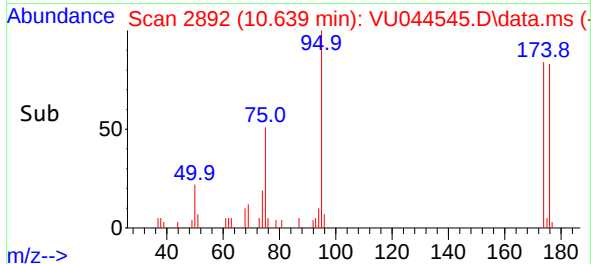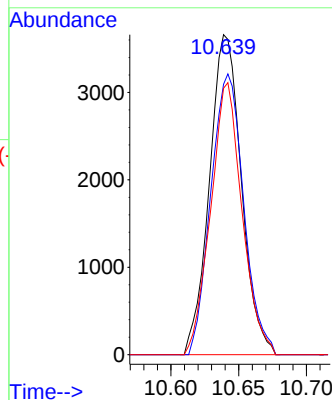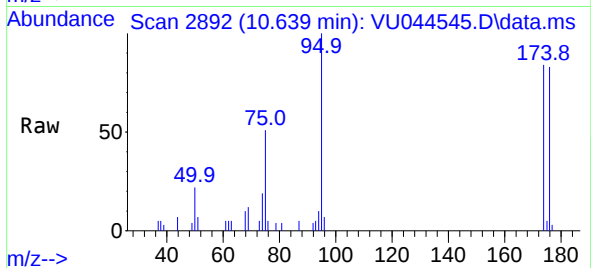

#68
1,2-Dichlorobenzene-d4
Concen: 0.815 ug/l
RT: 12.198 min Scan# 3377
Delta R.T. -0.000 min
Lab File: VU044545.D
Acq: 01 Sep 2021 12:31

Tgt Ion:152 Resp: 6824
Ion Ratio Lower Upper
152 100
115 64.5 0.0 277.8
150 169.2 0.0 674.2

