

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
 Data File : VU044543.D
 Acq On : 01 Sep 2021 10:27
 Operator : SY/MD
 Sample : VU0901WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0901WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.054	521	533	547	rBV	14746	29238	48.41%	14.589%
2	3.189	567	575	576	rBV4	2280	2574	4.26%	1.284%
3	6.121	1470	1487	1501	rBV	19951	37408	61.94%	18.666%
4	7.909	2035	2043	2049	rVB2	892	1534	2.54%	0.765%
5	8.478	2212	2220	2224	rBV3	554	707	1.17%	0.353%
6	8.658	2272	2276	2287	rVB6	706	825	1.37%	0.412%
7	8.944	2357	2365	2367	rBV4	942	1318	2.18%	0.658%
8	9.423	2502	2514	2526	rBV3	3581	6724	11.13%	3.355%
9	10.642	2883	2893	2905	rBV2	18606	29303	48.52%	14.622%
10	10.764	2923	2931	2941	rBV2	4619	6429	10.64%	3.208%
11	11.754	3233	3239	3246	rBV2	710	701	1.16%	0.350%
12	11.819	3250	3259	3272	rVV2	11362	19210	31.81%	9.585%
13	12.201	3364	3378	3395	rBV	36117	60397	100.00%	30.137%
14	13.848	3884	3890	3901	rBV3	707	1218	2.02%	0.608%
15	14.098	3959	3968	3977	rVB2	991	1640	2.72%	0.818%
16	14.343	4036	4044	4049	rVB2	872	1182	1.96%	0.590%




Sum of corrected areas: 200408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044543.D
Acq On : 01 Sep 2021 10:27
Operator : SY/MD
Sample : VU0901WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

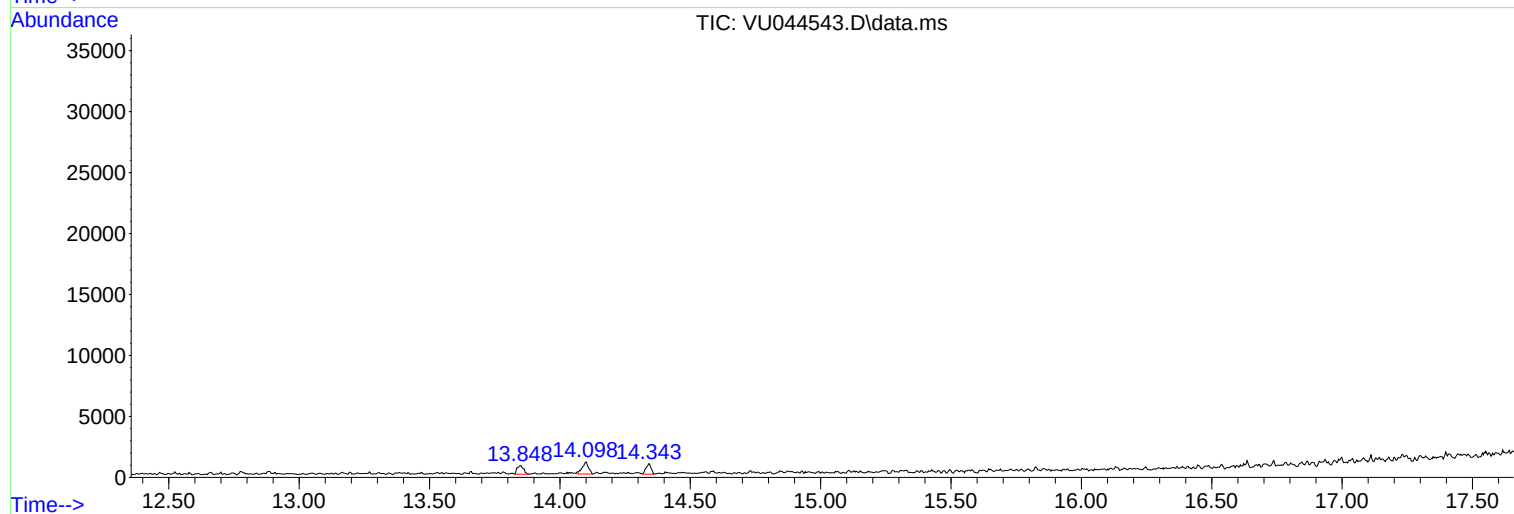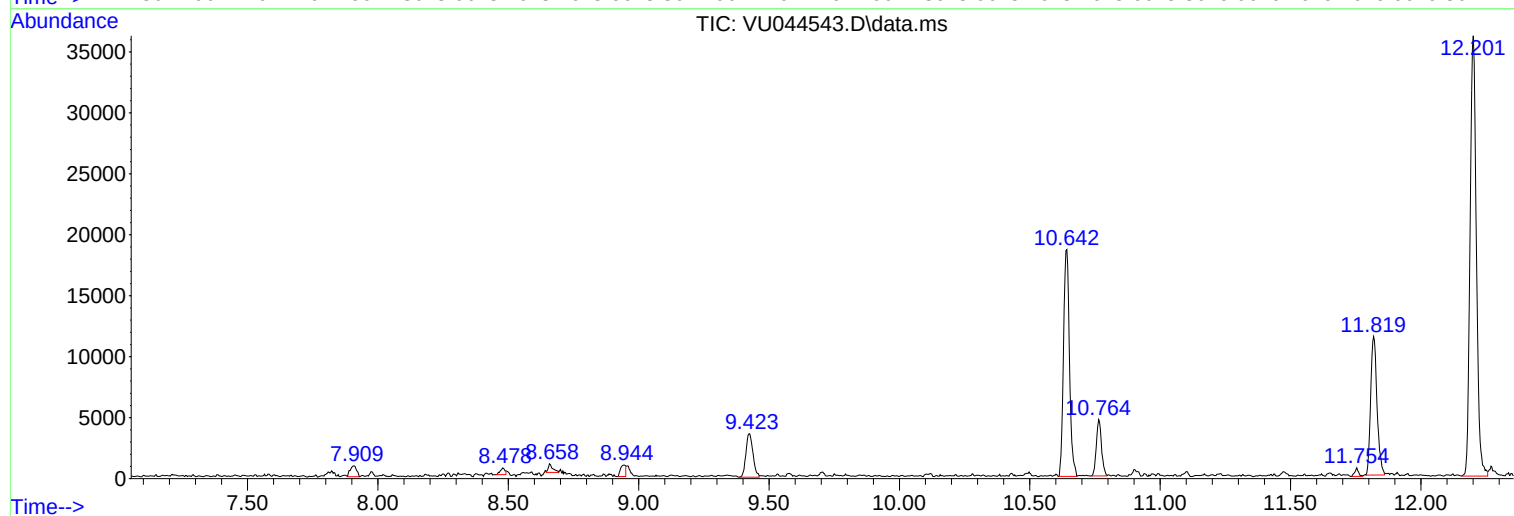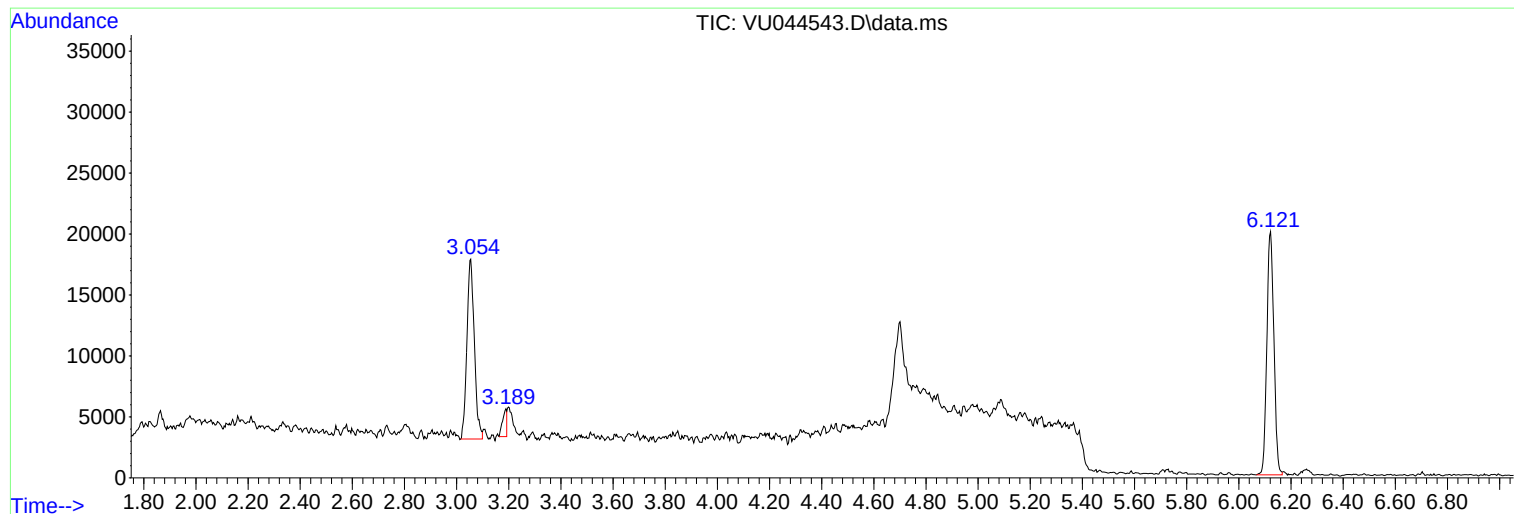

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044543.D
Acq On : 01 Sep 2021 10:27
Operator : SY/MD
Sample : VU0901WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044543.D
Acq On : 01 Sep 2021 10:27
Operator : SY/MD
Sample : VU0901WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0901WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------