

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
 Data File : VU044545.D
 Acq On : 01 Sep 2021 12:31
 Operator : SY/MD
 Sample : M3604-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-083021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.054	523	533	547	rVB2	14390	28340	71.44%	19.936%
2	3.700	729	734	746	rVB6	1508	2712	6.84%	1.908%
3	3.874	785	788	796	rVB4	770	609	1.54%	0.428%
4	3.964	814	816	821	rVB3	516	408	1.03%	0.287%
5	6.121	1474	1487	1502	rBV2	19917	36904	93.03%	25.960%
6	8.481	2213	2221	2229	rVB	666	1247	3.14%	0.877%
7	10.639	2882	2892	2904	rBV2	17587	27976	70.52%	19.680%
8	10.902	2968	2974	2983	rVB	760	1248	3.15%	0.878%
9	11.816	3246	3258	3259	rBV3	388	420	1.06%	0.295%
10	12.201	3365	3378	3389	rBV	24215	39670	100.00%	27.906%
11	14.102	3961	3969	3979	rVB2	660	1235	3.11%	0.869%
12	16.809	4806	4811	4816	rBV4	314	409	1.03%	0.288%
13	16.870	4825	4830	4834	rBV2	595	572	1.44%	0.402%
14	17.307	4963	4966	4971	rVB2	406	405	1.02%	0.285%




Sum of corrected areas: 142155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044545.D
Acq On : 01 Sep 2021 12:31
Operator : SY/MD
Sample : M3604-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

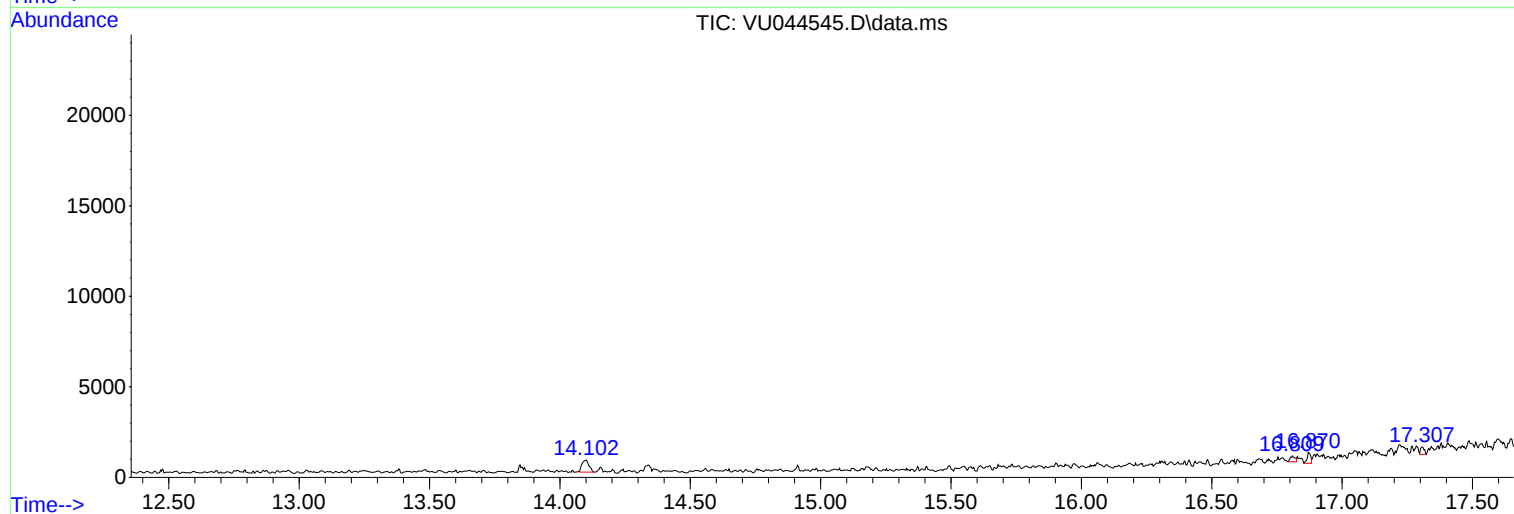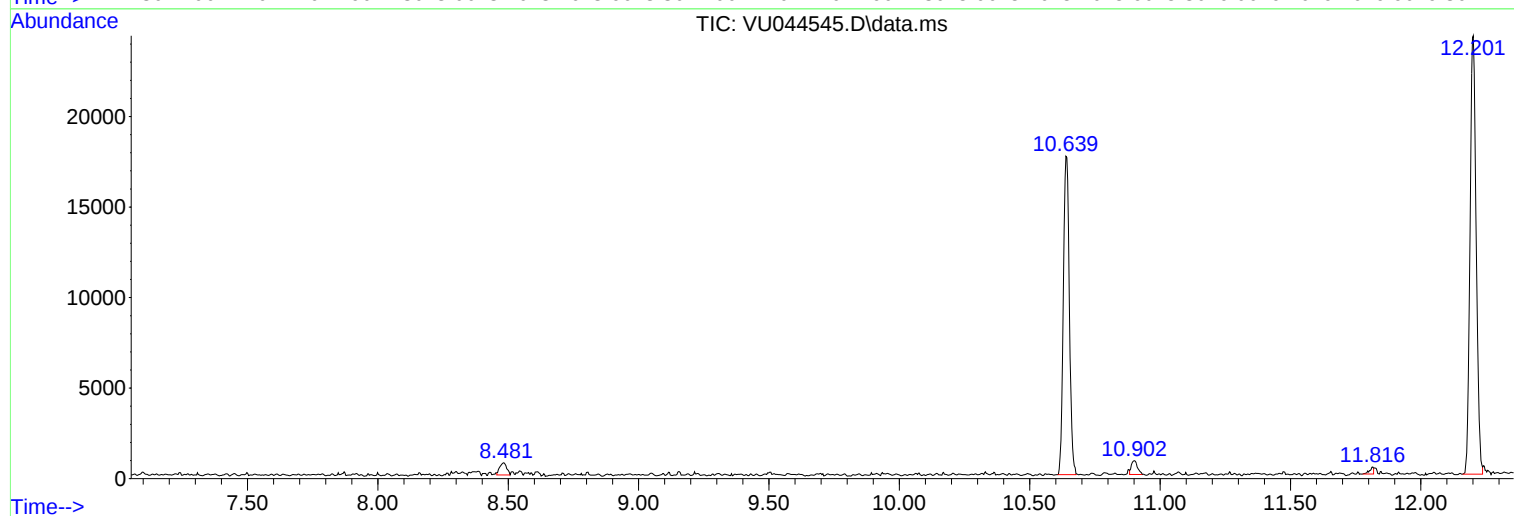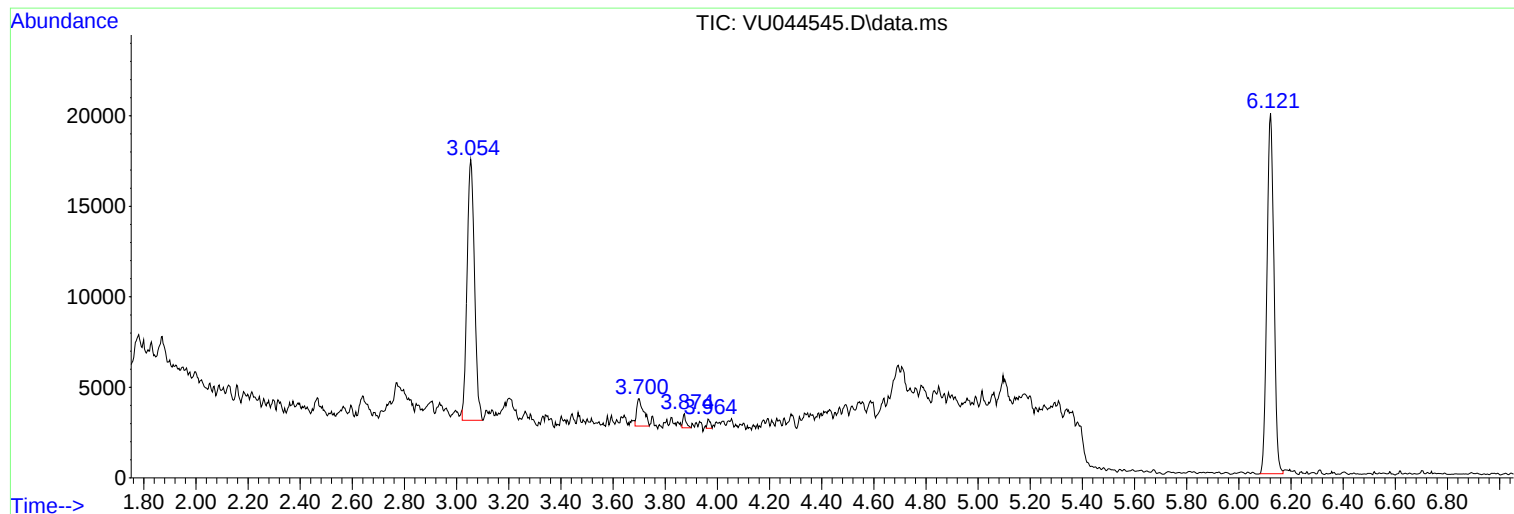

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044545.D
Acq On : 01 Sep 2021 12:31
Operator : SY/MD
Sample : M3604-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044545.D
Acq On : 01 Sep 2021 12:31
Operator : SY/MD
Sample : M3604-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------