

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044548.D
Acq On : 01 Sep 2021 14:01
Operator : SY/MD
Sample : M3586-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L66-082721-FD

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.096	1150	1168	1203	rBV	1353540	2917531	100.00%	91.259%
2	6.121	1474	1487	1500	rBV	18879	34801	1.19%	1.089%
3	7.115	1782	1796	1820	rBV	112517	208161	7.13%	6.511%
4	12.198	3366	3377	3390	rBV2	22885	36494	1.25%	1.142%




Sum of corrected areas: 3196987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044548.D
Acq On : 01 Sep 2021 14:01
Operator : SY/MD
Sample : M3586-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L66-082721-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

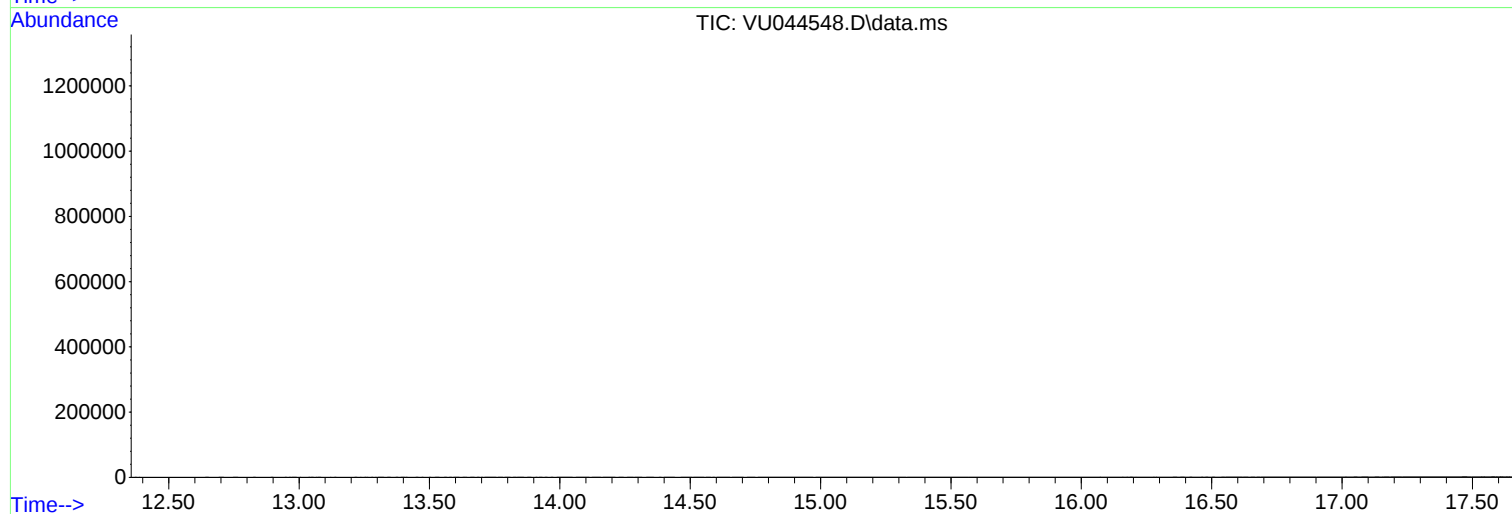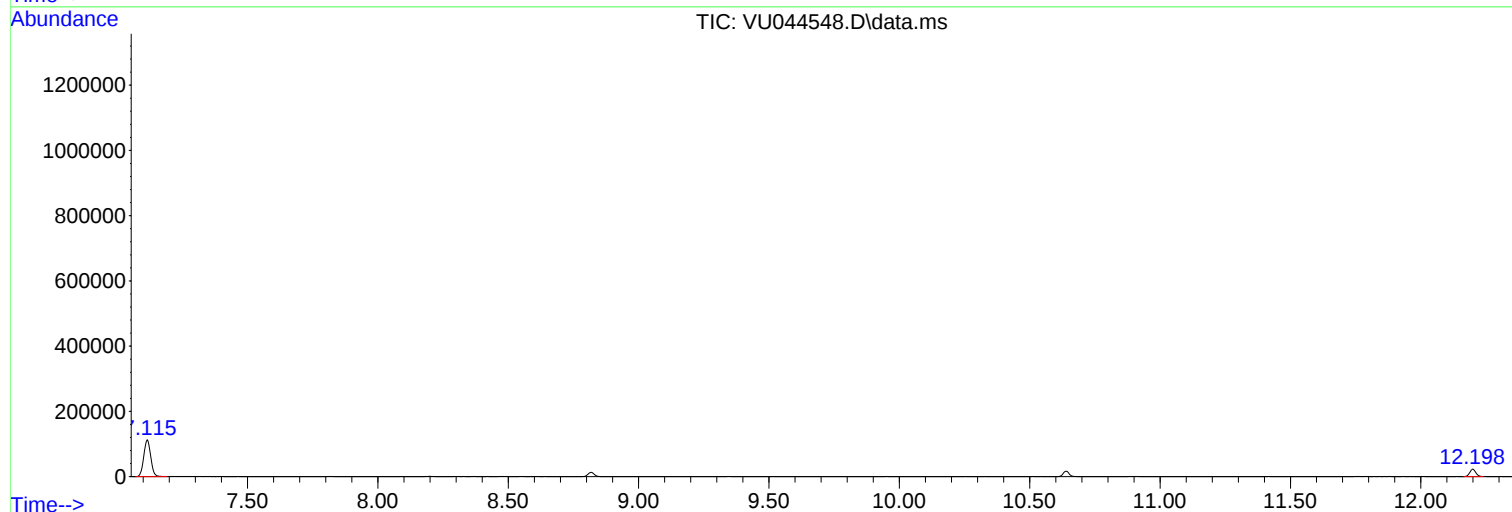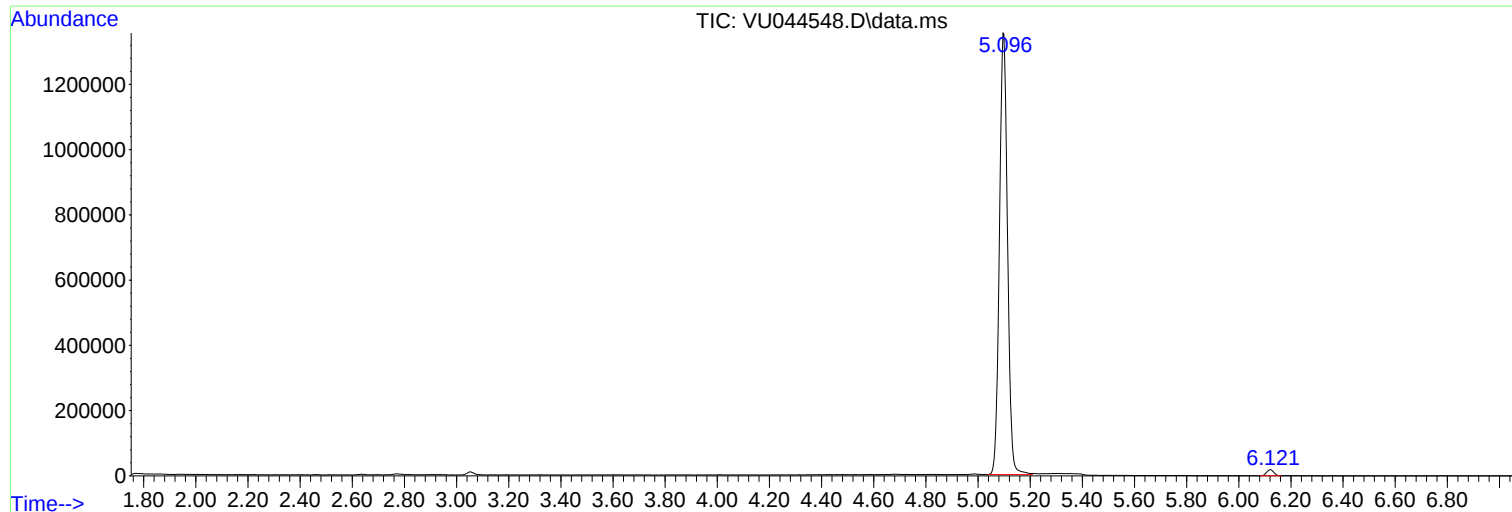

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044548.D
Acq On : 01 Sep 2021 14:01
Operator : SY/MD
Sample : M3586-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L66-082721-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044548.D
Acq On : 01 Sep 2021 14:01
Operator : SY/MD
Sample : M3586-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L66-082721-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard---			
					#	RT	Resp	Conc
