

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
 Data File : VU044549.D
 Acq On : 01 Sep 2021 14:31
 Operator : SY/MD
 Sample : M3604-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PW-B6-L41-083021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.587	380	388	397	rBV4	7508	12055	31.11%	5.271%
2	2.771	438	445	452	rBV2	3263	5934	15.31%	2.594%
3	3.054	525	533	541	rBV4	5938	9973	25.74%	4.360%
4	4.009	827	830	833	rBV3	707	481	1.24%	0.210%
5	4.677	1027	1038	1055	rVB4	15139	34717	89.59%	15.179%
6	5.086	1163	1165	1170	rBV4	1082	1047	2.70%	0.458%
7	5.777	1370	1380	1397	rVB2	3666	7264	18.75%	3.176%
8	6.121	1474	1487	1502	rBV	19449	36565	94.36%	15.987%
9	6.549	1610	1620	1632	rBV2	14451	25805	66.59%	11.283%
10	7.738	1987	1990	1996	rVB3	532	508	1.31%	0.222%
11	7.980	2060	2065	2075	rVB2	368	408	1.05%	0.178%
12	8.558	2236	2245	2256	rBV2	15415	24755	63.88%	10.824%
13	10.639	2882	2892	2905	rBV	17287	26580	68.59%	11.621%
14	10.899	2966	2973	2982	rVB3	557	803	2.07%	0.351%
15	12.198	3366	3377	3393	rBV2	24438	38751	100.00%	16.943%
16	14.101	3954	3969	3977	rVB	687	1511	3.90%	0.661%
17	16.934	4847	4850	4857	rVB3	429	518	1.34%	0.226%
18	16.973	4857	4862	4865	rBV	352	466	1.20%	0.204%
19	17.513	5026	5030	5034	rBV3	571	574	1.48%	0.251%




Sum of corrected areas: 228715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044549.D
Acq On : 01 Sep 2021 14:31
Operator : SY/MD
Sample : M3604-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L41-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

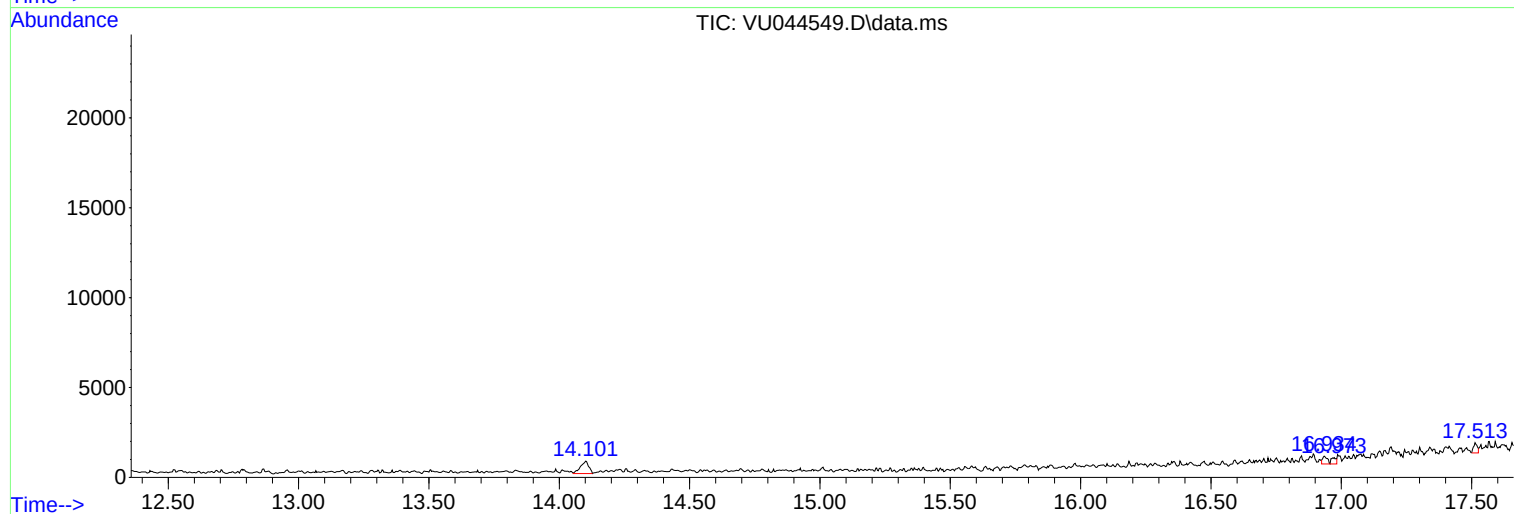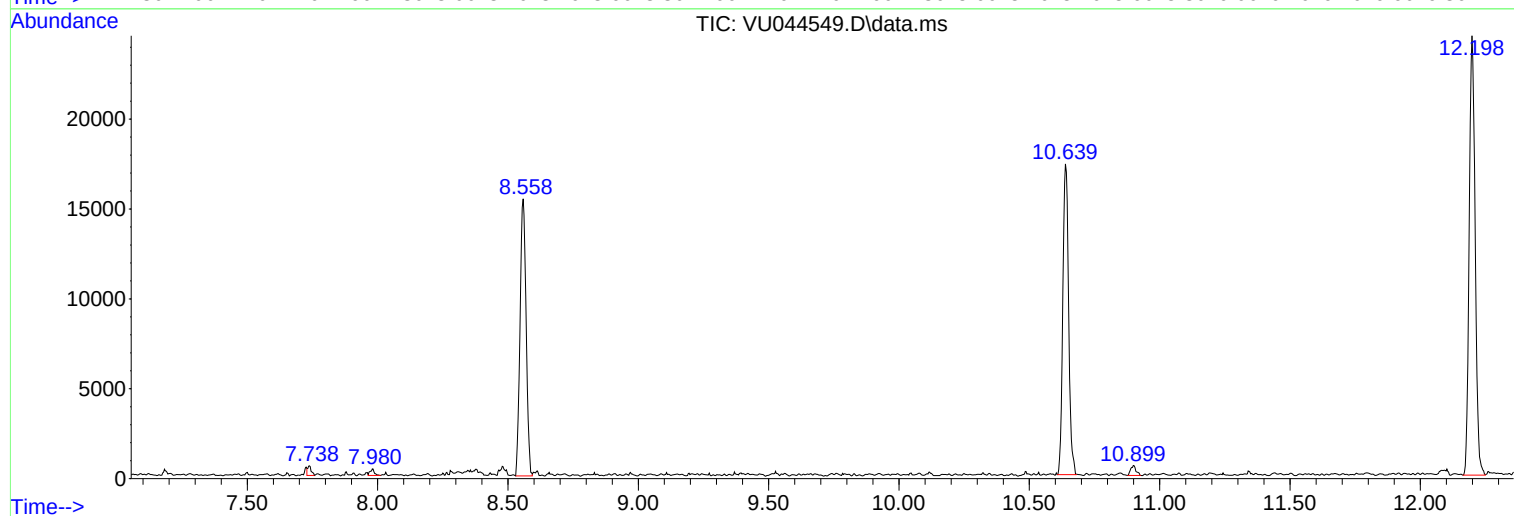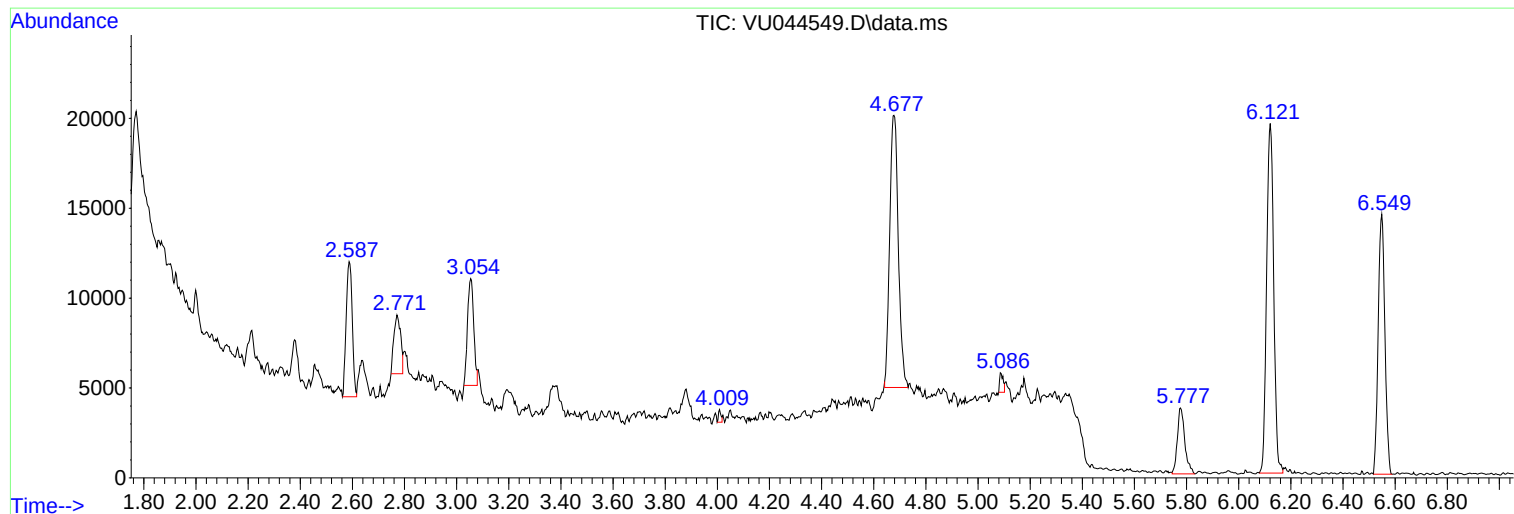

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044549.D
Acq On : 01 Sep 2021 14:31
Operator : SY/MD
Sample : M3604-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L41-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090121\
Data File : VU044549.D
Acq On : 01 Sep 2021 14:31
Operator : SY/MD
Sample : M3604-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PW-B6-L41-083021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U083121DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------