




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050588.D
 Acq On : 01 Sep 2022 18:07
 Operator : SY/MD
 Sample : N4362-08ME
 Misc : 5.40g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB9ME

Manual IntegrationsAPPROVED

Quant Time: Sep 02 02:10:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 02 02:07:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/05/2022

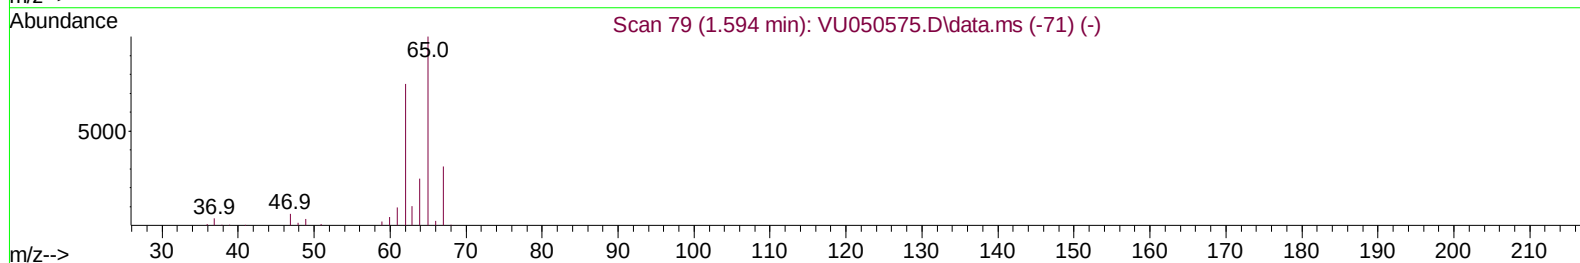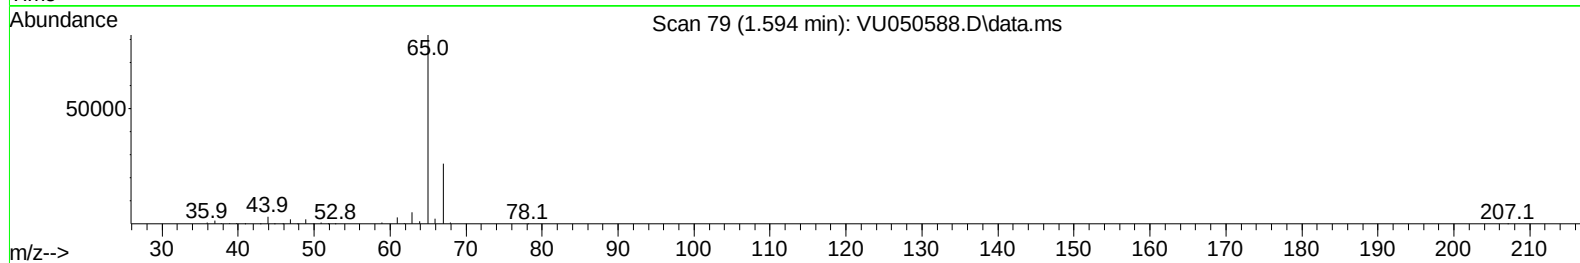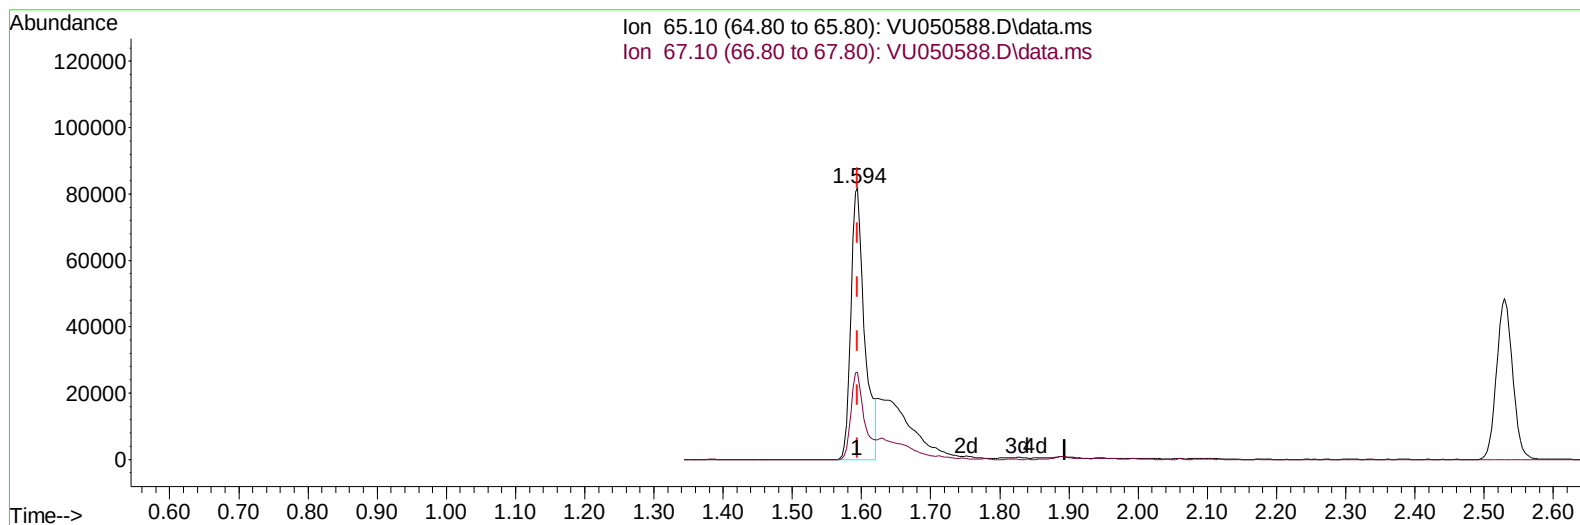

TIC: VU050588.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 25.75 ug/L

response 113423

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	31.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050588.D
 Acq On : 01 Sep 2022 18:07
 Operator : SY/MD
 Sample : N4362-08ME
 Misc : 5.40g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB9ME

Manual IntegrationsAPPROVED

Quant Time: Sep 02 02:10:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 02 02:07:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/05/2022

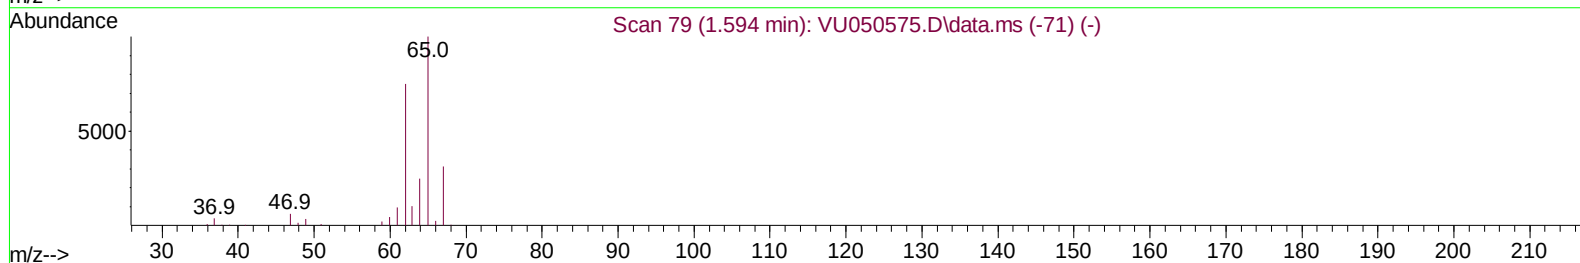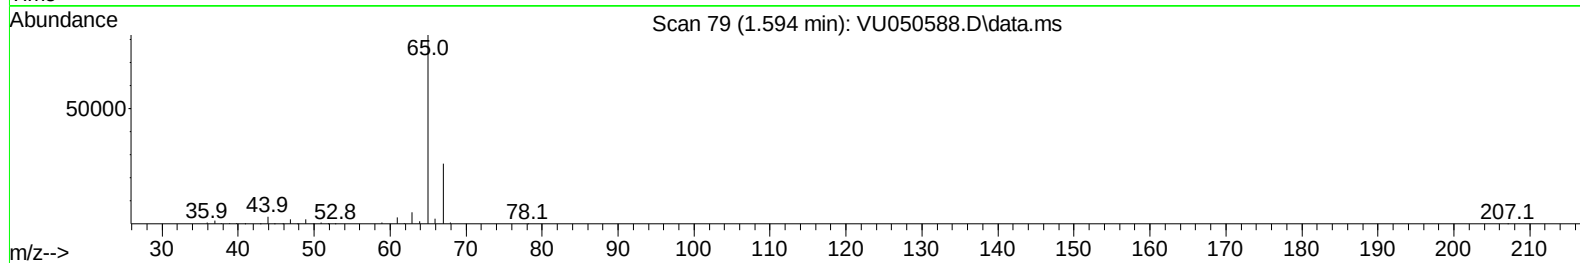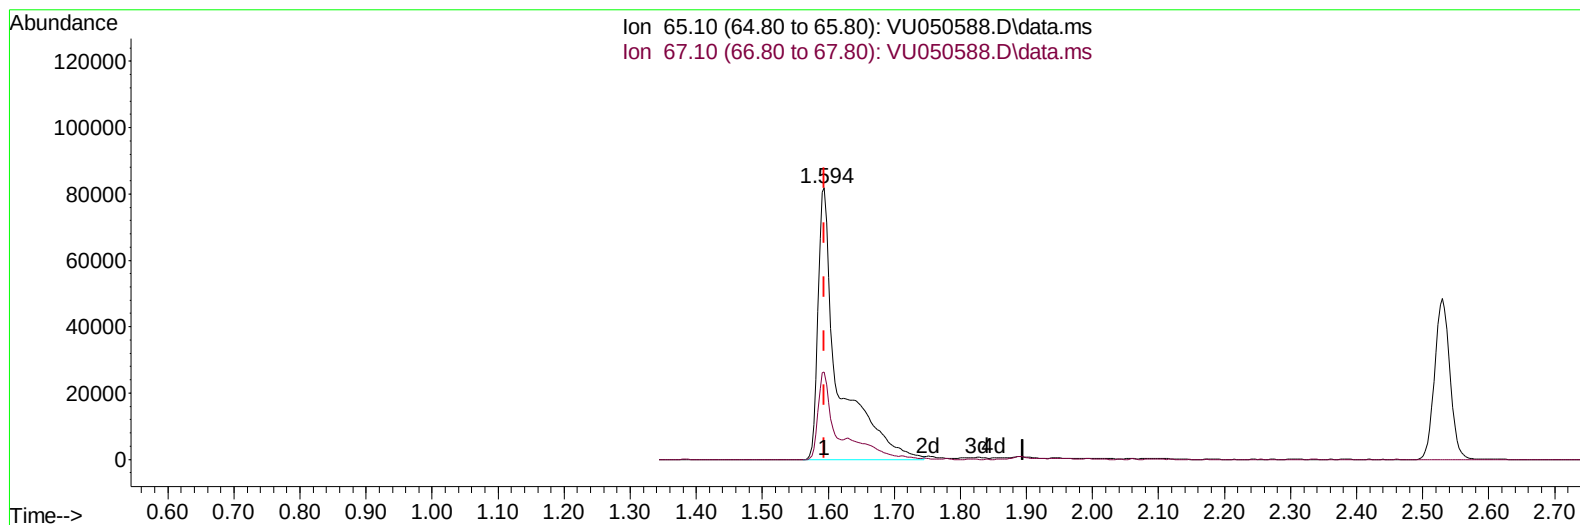

TIC: VU050588.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.000) 40.29 ug/L m

response 177440

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	20.36#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050588.D
 Acq On : 01 Sep 2022 18:07
 Operator : SY/MD
 Sample : N4362-08ME
 Misc : 5.40g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FB9ME

Manual IntegrationsAPPROVED

Quant Time: Sep 02 02:10:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 02 02:07:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	574206	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	378199	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	199521	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	177440m	40.291	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	80.580%	
7) Chloroethane-d5	1.890	69	65030	18.940	ug/L	-0.01
Spiked Amount 50.000	Range 70	- 130	Recovery	=	37.880%#	
11) 1,1-Dichloroethene-d2	2.530	63	247429	33.276	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	66.560%	
21) 2-Butanone-d5	4.645	46	331265	86.008	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	86.010%	
24) Chloroform-d	5.060	84	375203	43.785	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.580%	
26) 1,2-Dichloroethane-d4	5.700	65	245752	44.151	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.300%	
32) Benzene-d6	5.719	84	778202	66.388	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	132.780%#	
36) 1,2-Dichloropropane-d6	6.690	67	264051	67.653	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	135.300%#	
41) Toluene-d8	7.899	98	597801	58.621	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	117.240%	
43) trans-1,3-Dichloroprop...	8.179	79	76422	48.686	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	97.380%	
47) 2-Hexanone-d5	8.661	63	127142	89.969	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.970%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	377459	62.002	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	124.000%#	
66) 1,2-Dichlorobenzene-d4	12.195	152	205347	47.536	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.080%	
Target Compounds						
					Qvalue	
51) Chlorobenzene	9.452	112	10461	1.233	ug/L	95
65) 1,4-Dichlorobenzene	11.841	146	18840	2.737	ug/L	97
67) 1,2-Dichlorobenzene	12.214	146	22284	3.028	ug/L	96
70) 1,2,4-trichlorobenzene	13.848	180	10123	2.450	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050588.D
Acq On : 01 Sep 2022 18:07
Operator : SY/MD
Sample : N4362-08ME
Misc : 5.40g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FB9ME

Manual IntegrationsAPPROVED

Quant Time: Sep 02 02:10:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 02 02:07:32 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/05/2022

