

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050583.D
 Acq On : 01 Sep 2022 16:10
 Operator : SY/MD
 Sample : N4362-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Quant Time: Sep 02 02:09:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 02 02:07:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	252175	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	252702	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	89065	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	87792	45.392	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.780%		
7) Chloroethane-d5	1.903	69	68922	45.707	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.420%		
11) 1,1-Dichloroethene-d2	2.562	63	128880	39.467	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.940%		
21) 2-Butanone-d5	4.629	46	161695	95.593	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.590%		
24) Chloroform-d	5.063	84	214598	57.024	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	114.040%		
26) 1,2-Dichloroethane-d4	5.700	65	145361	59.464	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	118.920%		
32) Benzene-d6	5.726	84	422176	53.902	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	107.800%		
36) 1,2-Dichloropropane-d6	6.690	67	143701	55.103	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	110.200%		
41) Toluene-d8	7.899	98	344529	50.563	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.120%		
43) trans-1,3-Dichloroprop...	8.179	79	56981	54.329	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	108.660%		
47) 2-Hexanone-d5	8.636	63	67445	71.428	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	71.430%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	209047	51.392	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	102.780%		
66) 1,2-Dichlorobenzene-d4	12.192	152	113117	58.660	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	117.320%		
Target Compounds					Qvalue	
13) Acetone	2.639	43	7115	5.415	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050583.D
Acq On : 01 Sep 2022 16:10
Operator : SY/MD
Sample : N4362-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC2

Quant Time: Sep 02 02:09:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 02 02:07:32 2022
Response via : Initial Calibration

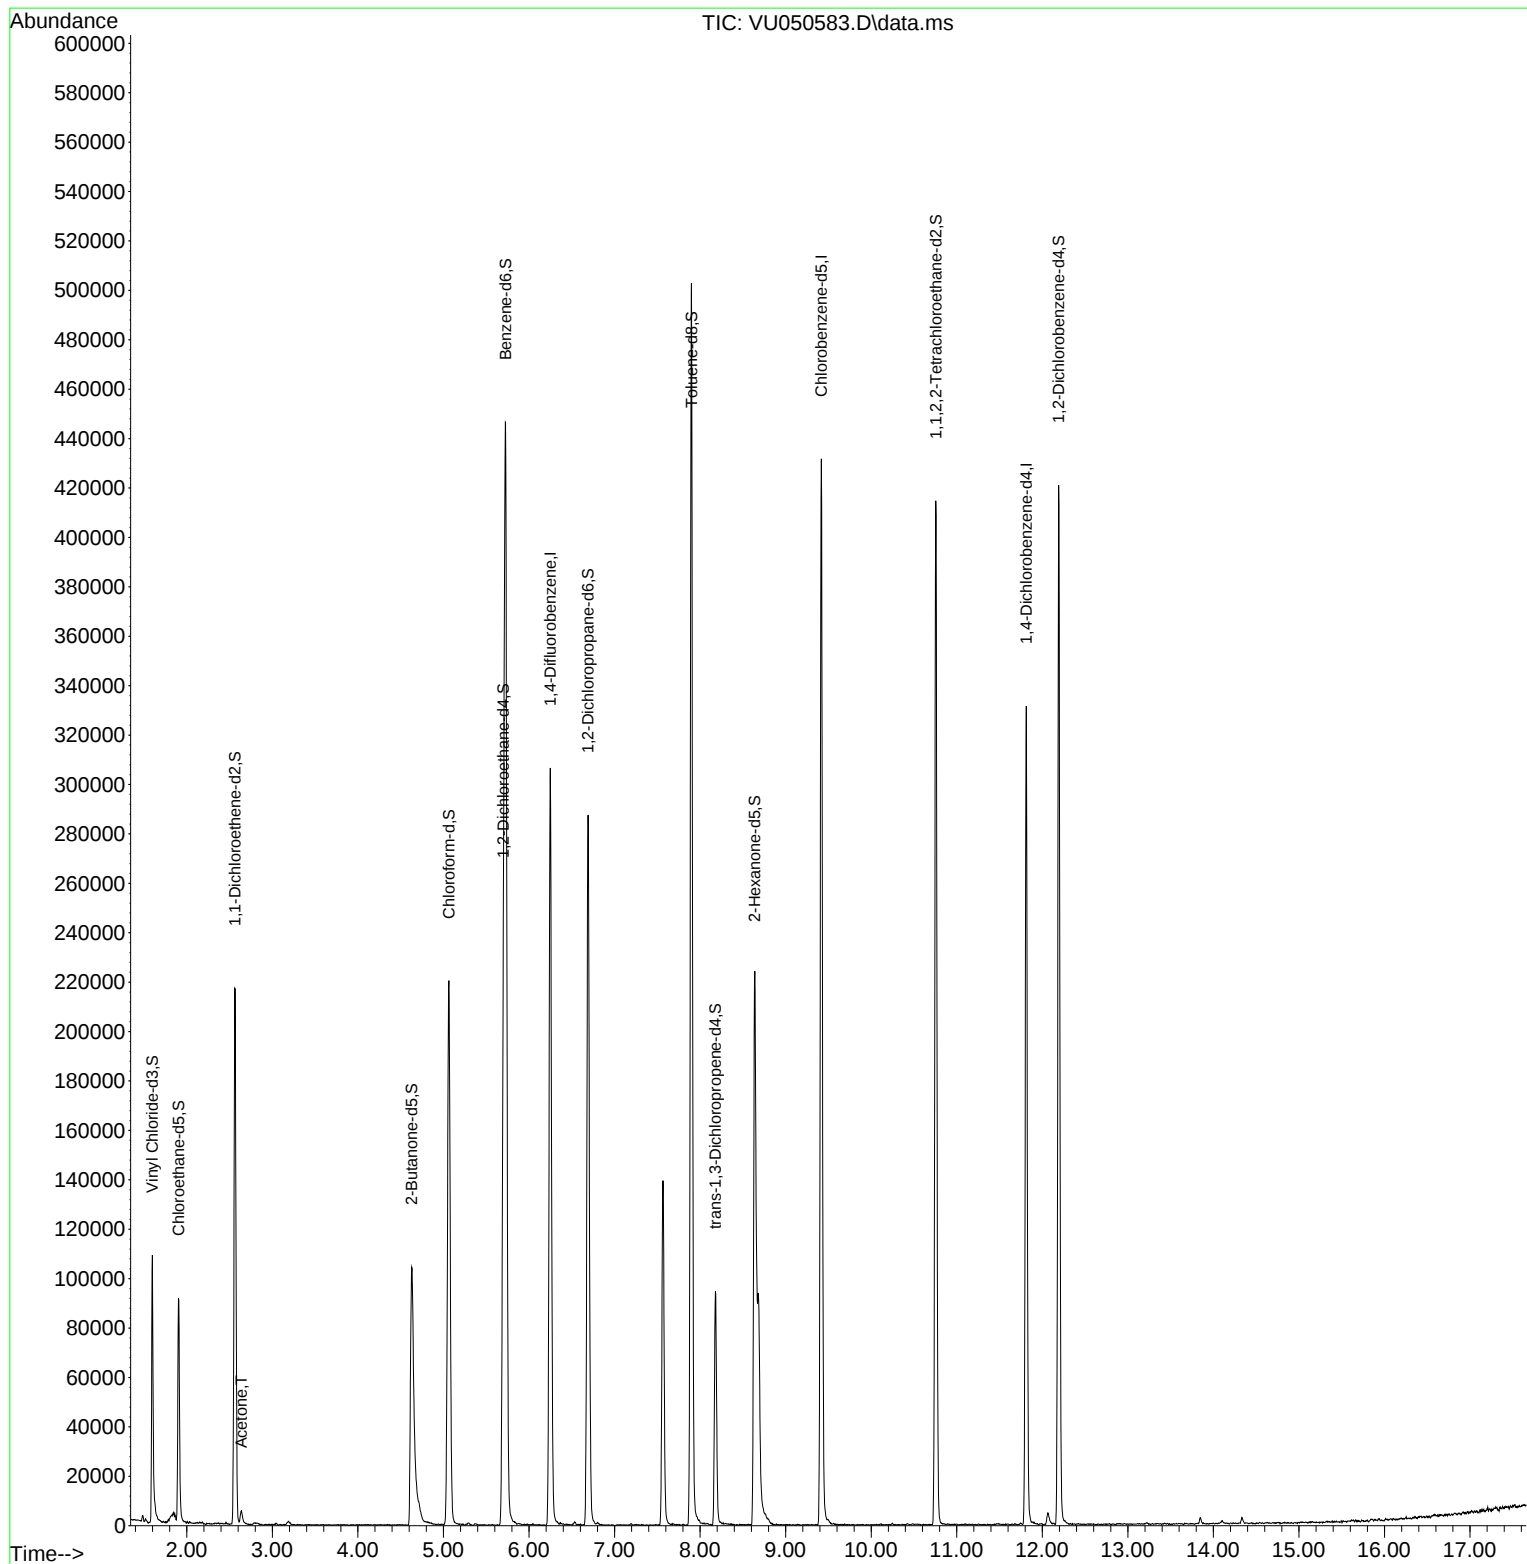

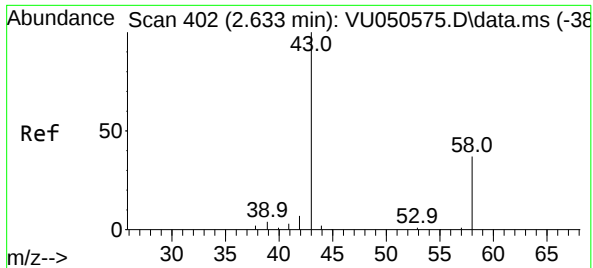

#13
 Acetone
 Concen: 5.415 ug/L
 RT: 2.639 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU050583.D
 Acq: 01 Sep 2022 16:10

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Tgt Ion: 43 Resp: 7115
 Ion Ratio Lower Upper
 43 100
 58 33.8 0.0 71.6

