

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050580.D
 Acq On : 01 Sep 2022 14:59
 Operator : SY/MD
 Sample : N4458-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COKW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rBV	111979	139659	6.09%	1.309%
2	1.729	116	121	130	rVB2	6087	7152	0.31%	0.067%
3	1.906	167	176	193	rVB	88891	119856	5.23%	1.123%
4	2.478	351	354	356	rBV2	352	245	0.01%	0.002%
5	2.565	368	381	394	rBV	213062	341424	14.90%	3.200%
6	2.745	434	437	439	rBV	363	250	0.01%	0.002%
7	2.900	482	485	488	rVB2	314	171	0.01%	0.002%
8	2.973	505	508	516	rBV2	231	243	0.01%	0.002%
9	3.041	527	529	532	rBV	538	396	0.02%	0.004%
10	3.121	549	554	558	rBV2	199	204	0.01%	0.002%
11	3.186	558	574	590	rBV	25955	60209	2.63%	0.564%
12	3.343	619	623	625	rBV2	291	264	0.01%	0.002%
13	3.436	646	652	654	rBV2	243	251	0.01%	0.002%
14	3.575	691	695	698	rVB2	285	240	0.01%	0.002%
15	3.613	703	707	710	rVB	296	252	0.01%	0.002%
16	3.633	710	713	717	rBV2	234	215	0.01%	0.002%
17	3.710	734	737	742	rBV	206	206	0.01%	0.002%
18	3.883	787	791	793	rVB	224	143	0.01%	0.001%
19	3.899	793	796	798	rBV2	213	141	0.01%	0.001%
20	3.945	807	810	817	rVB2	243	229	0.01%	0.002%
21	3.977	817	820	823	rBV	213	222	0.01%	0.002%
22	4.038	835	839	843	rBV2	288	274	0.01%	0.003%
23	4.063	843	847	850	rBV2	179	136	0.01%	0.001%
24	4.256	903	907	910	rBV	194	131	0.01%	0.001%
25	4.353	934	937	940	rBV2	235	183	0.01%	0.002%
26	4.372	940	943	951	rVB2	188	252	0.01%	0.002%
27	4.440	961	964	967	rBV2	180	141	0.01%	0.001%
28	4.456	967	969	974	rVB	273	229	0.01%	0.002%
29	4.481	974	977	980	rBV2	170	142	0.01%	0.001%
30	4.562	996	1002	1005	rBV2	248	251	0.01%	0.002%
31	4.629	1008	1023	1060	rBV3	113089	356213	15.54%	3.339%
32	5.063	1141	1158	1181	rBV	213650	469635	20.49%	4.402%
33	5.292	1219	1229	1236	rBV2	1047	1687	0.07%	0.016%
34	5.362	1249	1251	1252	rBV	365	158	0.01%	0.001%
35	5.424	1267	1270	1272	rVB	232	138	0.01%	0.001%
36	5.581	1314	1319	1325	rBV2	286	379	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050580.D
 Acq On : 01 Sep 2022 14:59
 Operator : SY/MD
 Sample : N4458-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COKW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	5.723	1338	1363	1396	rBV2	432446	1196893	52.22%	11.218%
38	5.944	1429	1432	1435	rBV2	226	143	0.01%	0.001%
39	5.996	1445	1448	1450	rBV	369	214	0.01%	0.002%
40	6.034	1457	1460	1462	rBV2	261	171	0.01%	0.002%
41	6.105	1479	1482	1485	rBV3	423	236	0.01%	0.002%
42	6.247	1512	1526	1545	rBV	293479	562429	24.54%	5.272%
43	6.491	1598	1602	1605	rBV	275	242	0.01%	0.002%
44	6.520	1607	1611	1613	rBV2	694	494	0.02%	0.005%
45	6.690	1648	1664	1688	rBV	275271	539745	23.55%	5.059%
46	6.806	1696	1700	1704	rBV4	781	813	0.04%	0.008%
47	6.867	1714	1719	1724	rBV2	345	406	0.02%	0.004%
48	6.951	1743	1745	1749	rBV2	183	137	0.01%	0.001%
49	7.002	1759	1761	1766	rVB	229	170	0.01%	0.002%
50	7.028	1766	1769	1771	rBV	222	149	0.01%	0.001%
51	7.079	1783	1785	1788	rBV	397	255	0.01%	0.002%
52	7.115	1793	1796	1802	rVB	283	328	0.01%	0.003%
53	7.182	1814	1817	1819	rBV2	756	437	0.02%	0.004%
54	7.440	1893	1897	1900	rVB	203	135	0.01%	0.001%
55	7.501	1911	1916	1924	rBV2	318	473	0.02%	0.004%
56	7.565	1924	1936	1956	rBV	136155	243536	10.63%	2.283%
57	7.758	1994	1996	2000	rBV	315	190	0.01%	0.002%
58	7.899	2026	2040	2076	rBV	493032	864167	37.70%	8.100%
59	8.179	2115	2127	2144	rBV2	92053	160111	6.99%	1.501%
60	8.465	2214	2216	2218	rBV	387	143	0.01%	0.001%
61	8.481	2218	2221	2230	rVB2	273	342	0.01%	0.003%
62	8.539	2236	2239	2241	rBV	199	131	0.01%	0.001%
63	8.639	2257	2270	2280	rBV3	206637	458723	20.01%	4.300%
64	8.877	2342	2344	2347	rBV	366	285	0.01%	0.003%
65	8.915	2353	2356	2360	rBV2	309	301	0.01%	0.003%
66	8.983	2375	2377	2383	rBV2	230	200	0.01%	0.002%
67	9.073	2400	2405	2408	rBV2	250	269	0.01%	0.003%
68	9.095	2410	2412	2417	rVB2	312	246	0.01%	0.002%
69	9.118	2417	2419	2423	rBV	221	140	0.01%	0.001%
70	9.195	2440	2443	2445	rBV	234	162	0.01%	0.002%
71	9.417	2499	2512	2518	rBV	436906	763193	33.30%	7.153%
72	9.603	2568	2570	2572	rBV	236	127	0.01%	0.001%
73	9.693	2594	2598	2601	rBV2	359	258	0.01%	0.002%
74	10.083	2715	2719	2721	rBV2	254	227	0.01%	0.002%
75	10.240	2766	2768	2776	rBV	281	375	0.02%	0.004%
76	10.391	2811	2815	2818	rBV2	281	266	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050580.D
 Acq On : 01 Sep 2022 14:59
 Operator : SY/MD
 Sample : N4458-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.648	2892	2895	2896	rBV2	252	133	0.01%	0.001%
78	10.697	2907	2910	2915	rBV2	243	252	0.01%	0.002%
79	10.755	2915	2928	2947	rBV	395259	643742	28.09%	6.034%
80	10.931	2981	2983	2985	rBV	294	175	0.01%	0.002%
81	11.092	3026	3033	3035	rBV4	610	621	0.03%	0.006%
82	11.150	3047	3051	3055	rBV2	220	208	0.01%	0.002%
83	11.472	3144	3151	3157	rVB2	860	1067	0.05%	0.010%
84	11.578	3181	3184	3187	rBV2	269	188	0.01%	0.002%
85	11.623	3194	3198	3199	rBV2	227	144	0.01%	0.001%
86	11.745	3226	3236	3245	rBV2	33820	53492	2.33%	0.501%
87	11.812	3246	3257	3285	rVB2	366195	852968	37.22%	7.995%
88	12.028	3322	3324	3330	rVB2	355	195	0.01%	0.002%
89	12.208	3361	3380	3410	rBV2	1066017	2291993	100.00%	21.482%
90	12.398	3435	3439	3443	rBV3	315	323	0.01%	0.003%
91	12.426	3443	3448	3451	rBV	451	495	0.02%	0.005%
92	12.578	3490	3495	3500	rBV3	421	523	0.02%	0.005%
93	12.684	3524	3528	3531	rBV	381	273	0.01%	0.003%
94	13.060	3641	3645	3648	rBV2	559	457	0.02%	0.004%
95	13.108	3658	3660	3666	rBV2	369	405	0.02%	0.004%
96	13.153	3672	3674	3679	rVB2	369	270	0.01%	0.003%
97	13.211	3681	3692	3704	rVV2	15732	29752	1.30%	0.279%
98	13.838	3876	3887	3907	rBV	182442	304938	13.30%	2.858%
99	14.089	3960	3965	3974	rVB2	4106	5269	0.23%	0.049%
100	14.330	4029	4040	4056	rBV	112387	182143	7.95%	1.707%




Sum of corrected areas: 10669209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050580.D
Acq On : 01 Sep 2022 14:59
Operator : SY/MD
Sample : N4458-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COKW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

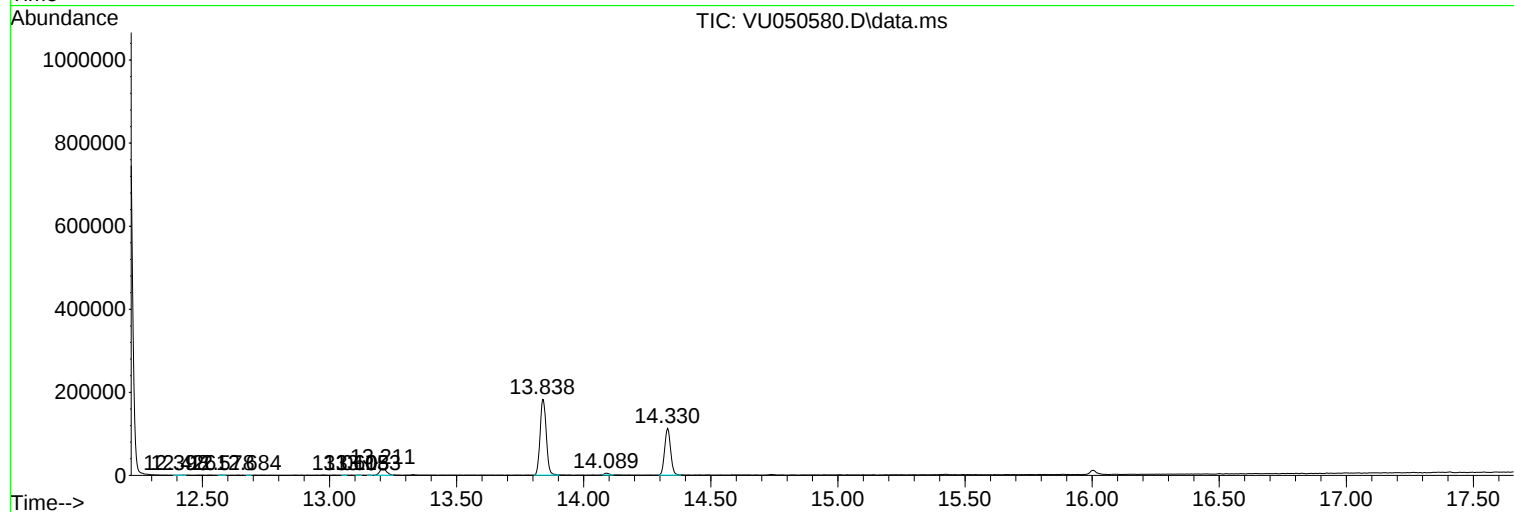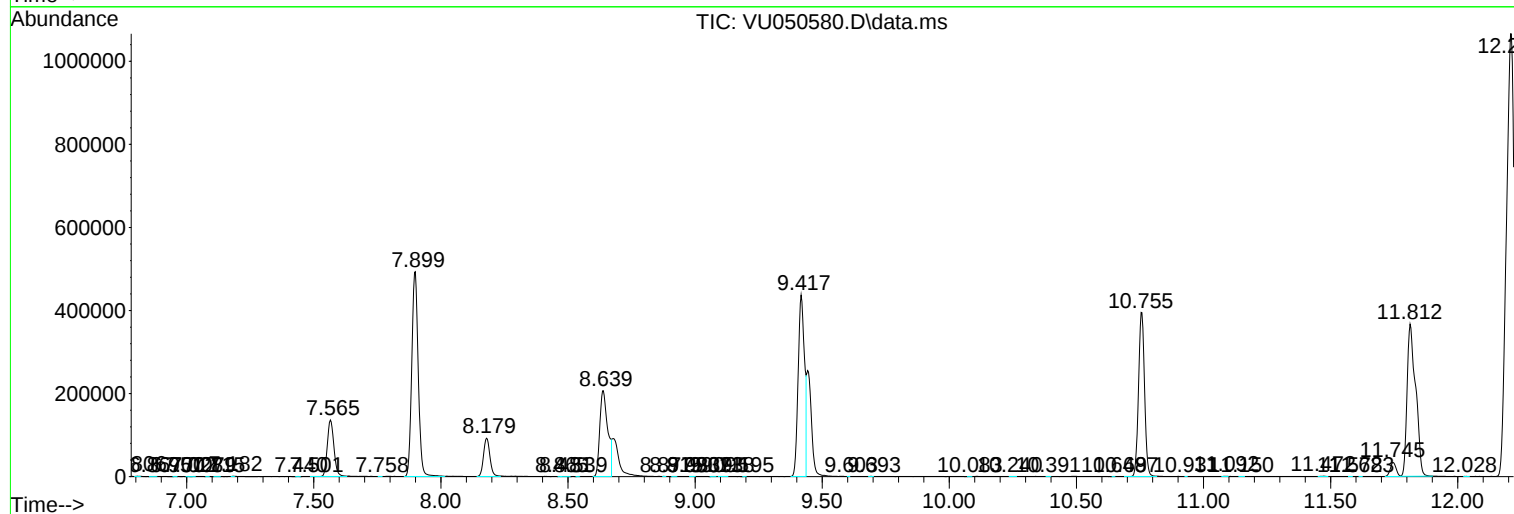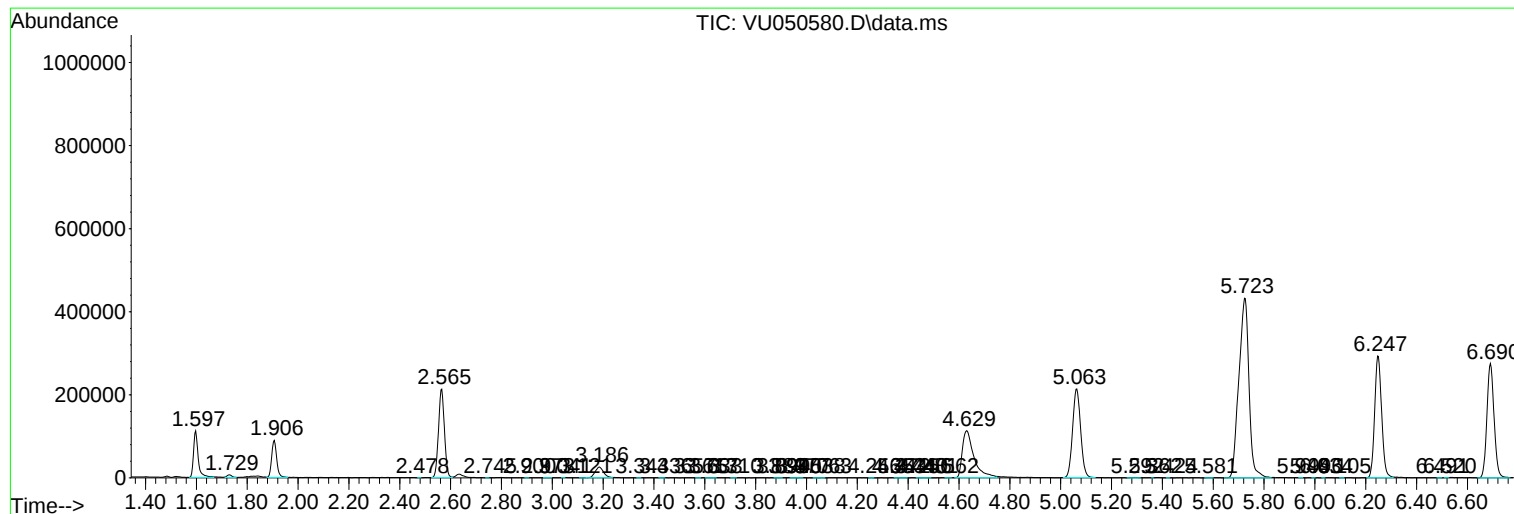

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050580.D
Acq On : 01 Sep 2022 14:59
Operator : SY/MD
Sample : N4458-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050580.D
Acq On : 01 Sep 2022 14:59
Operator : SY/MD
Sample : N4458-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc